
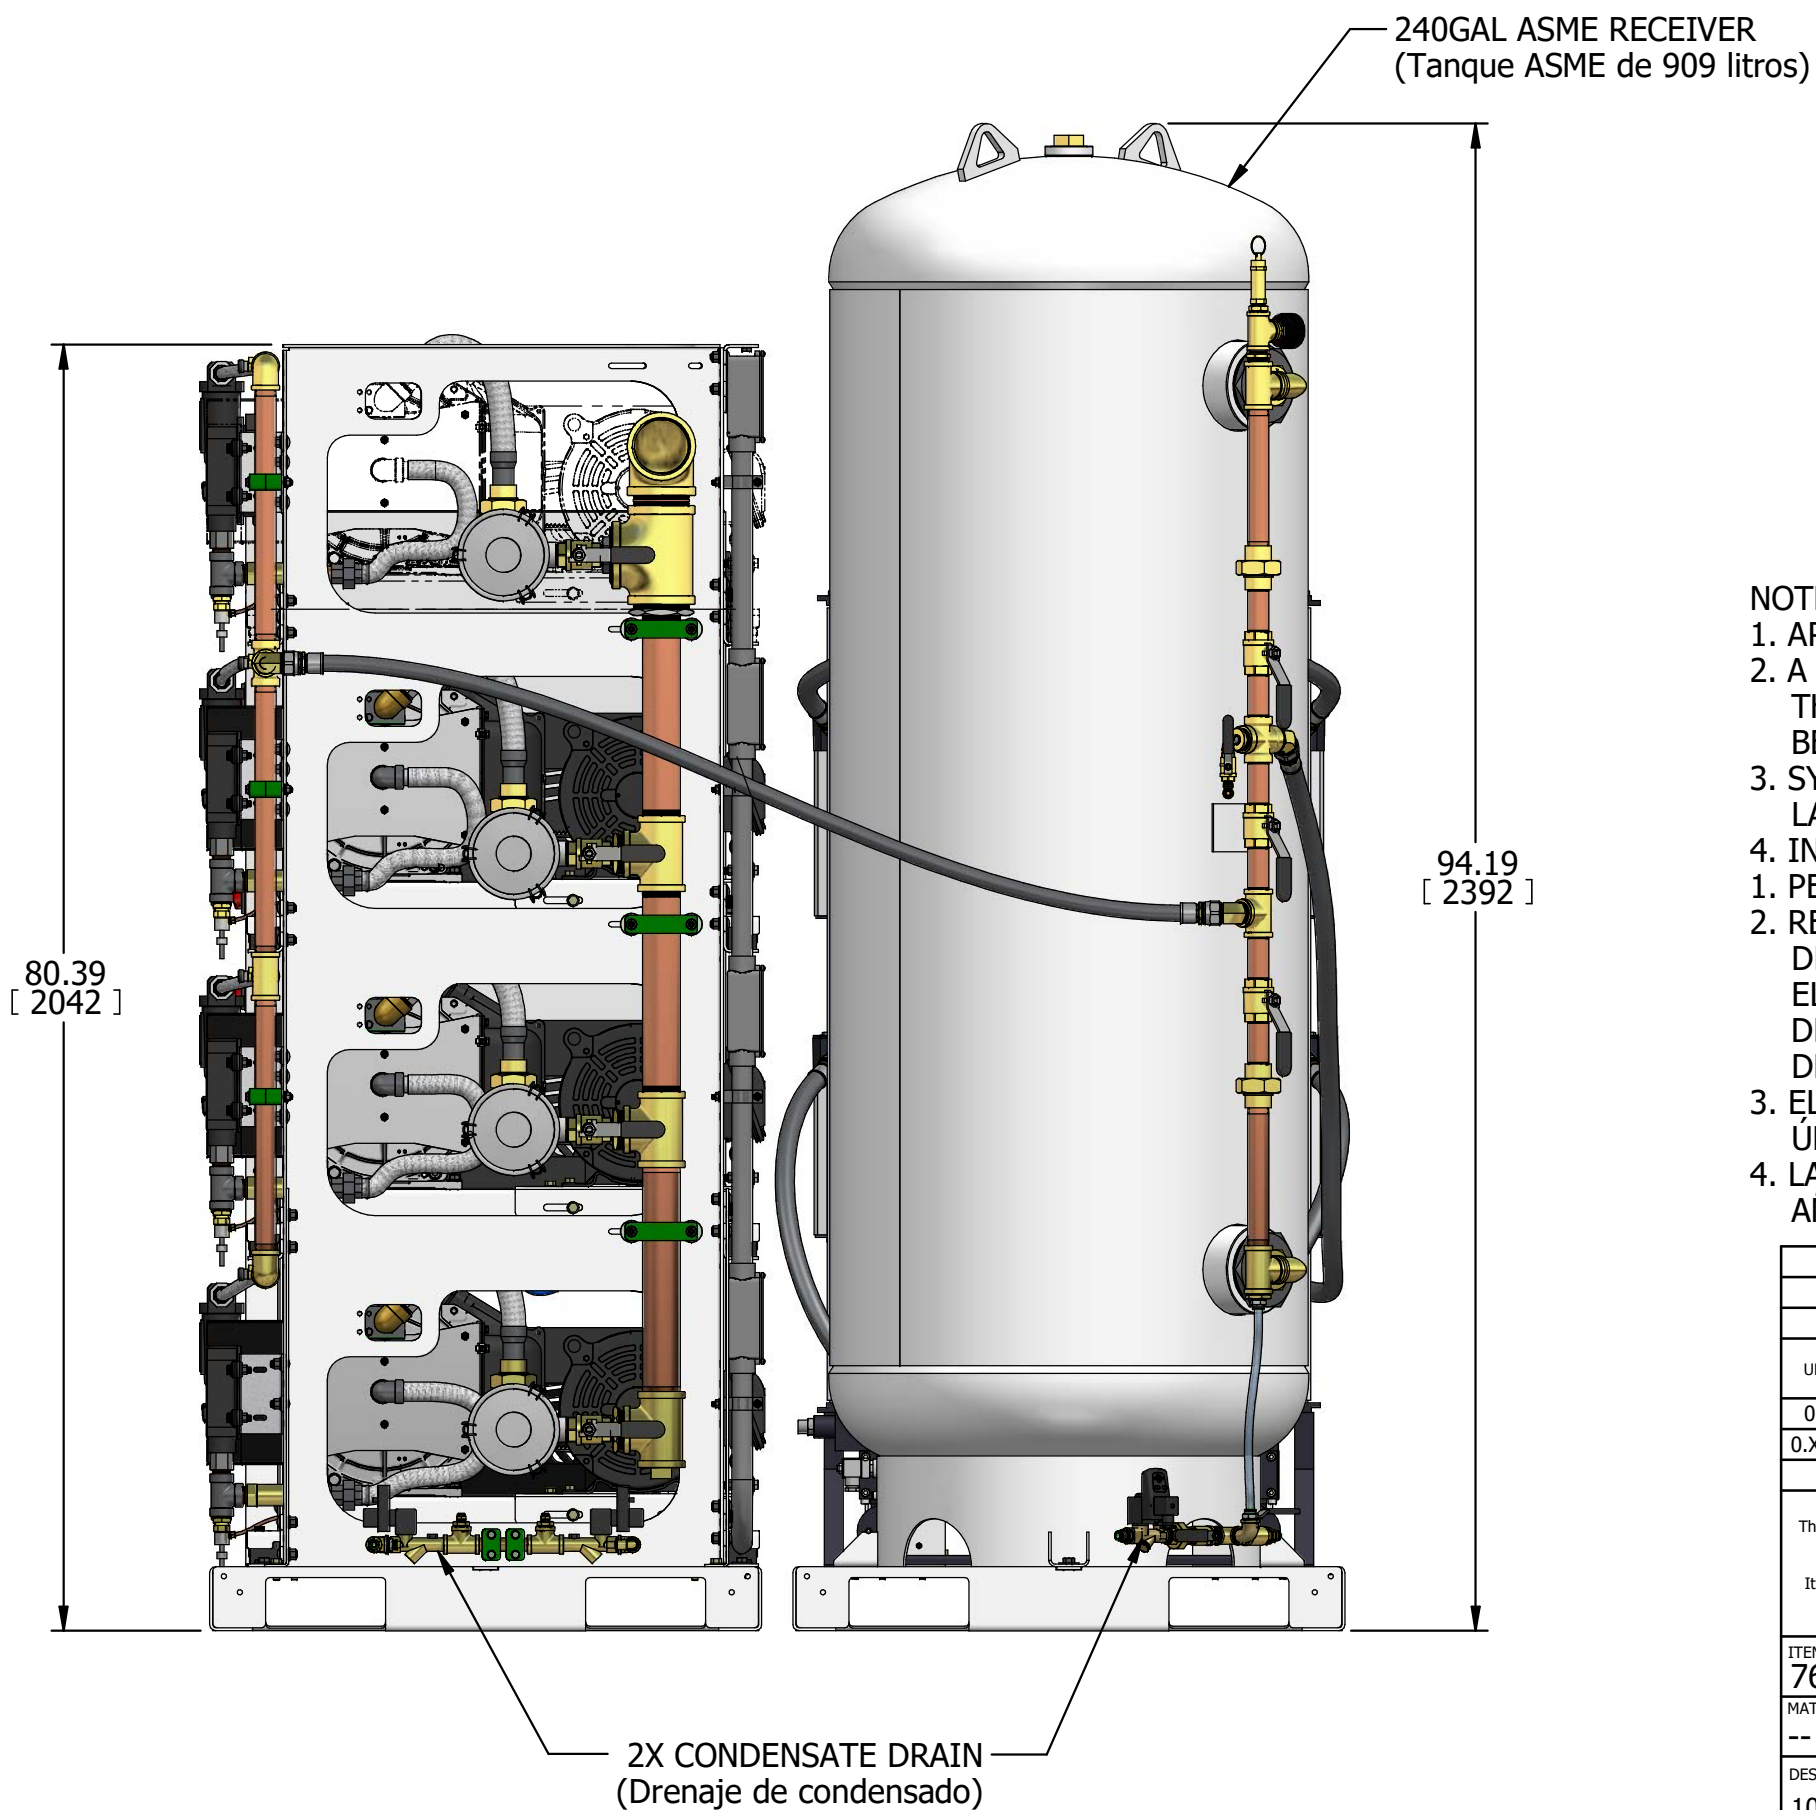
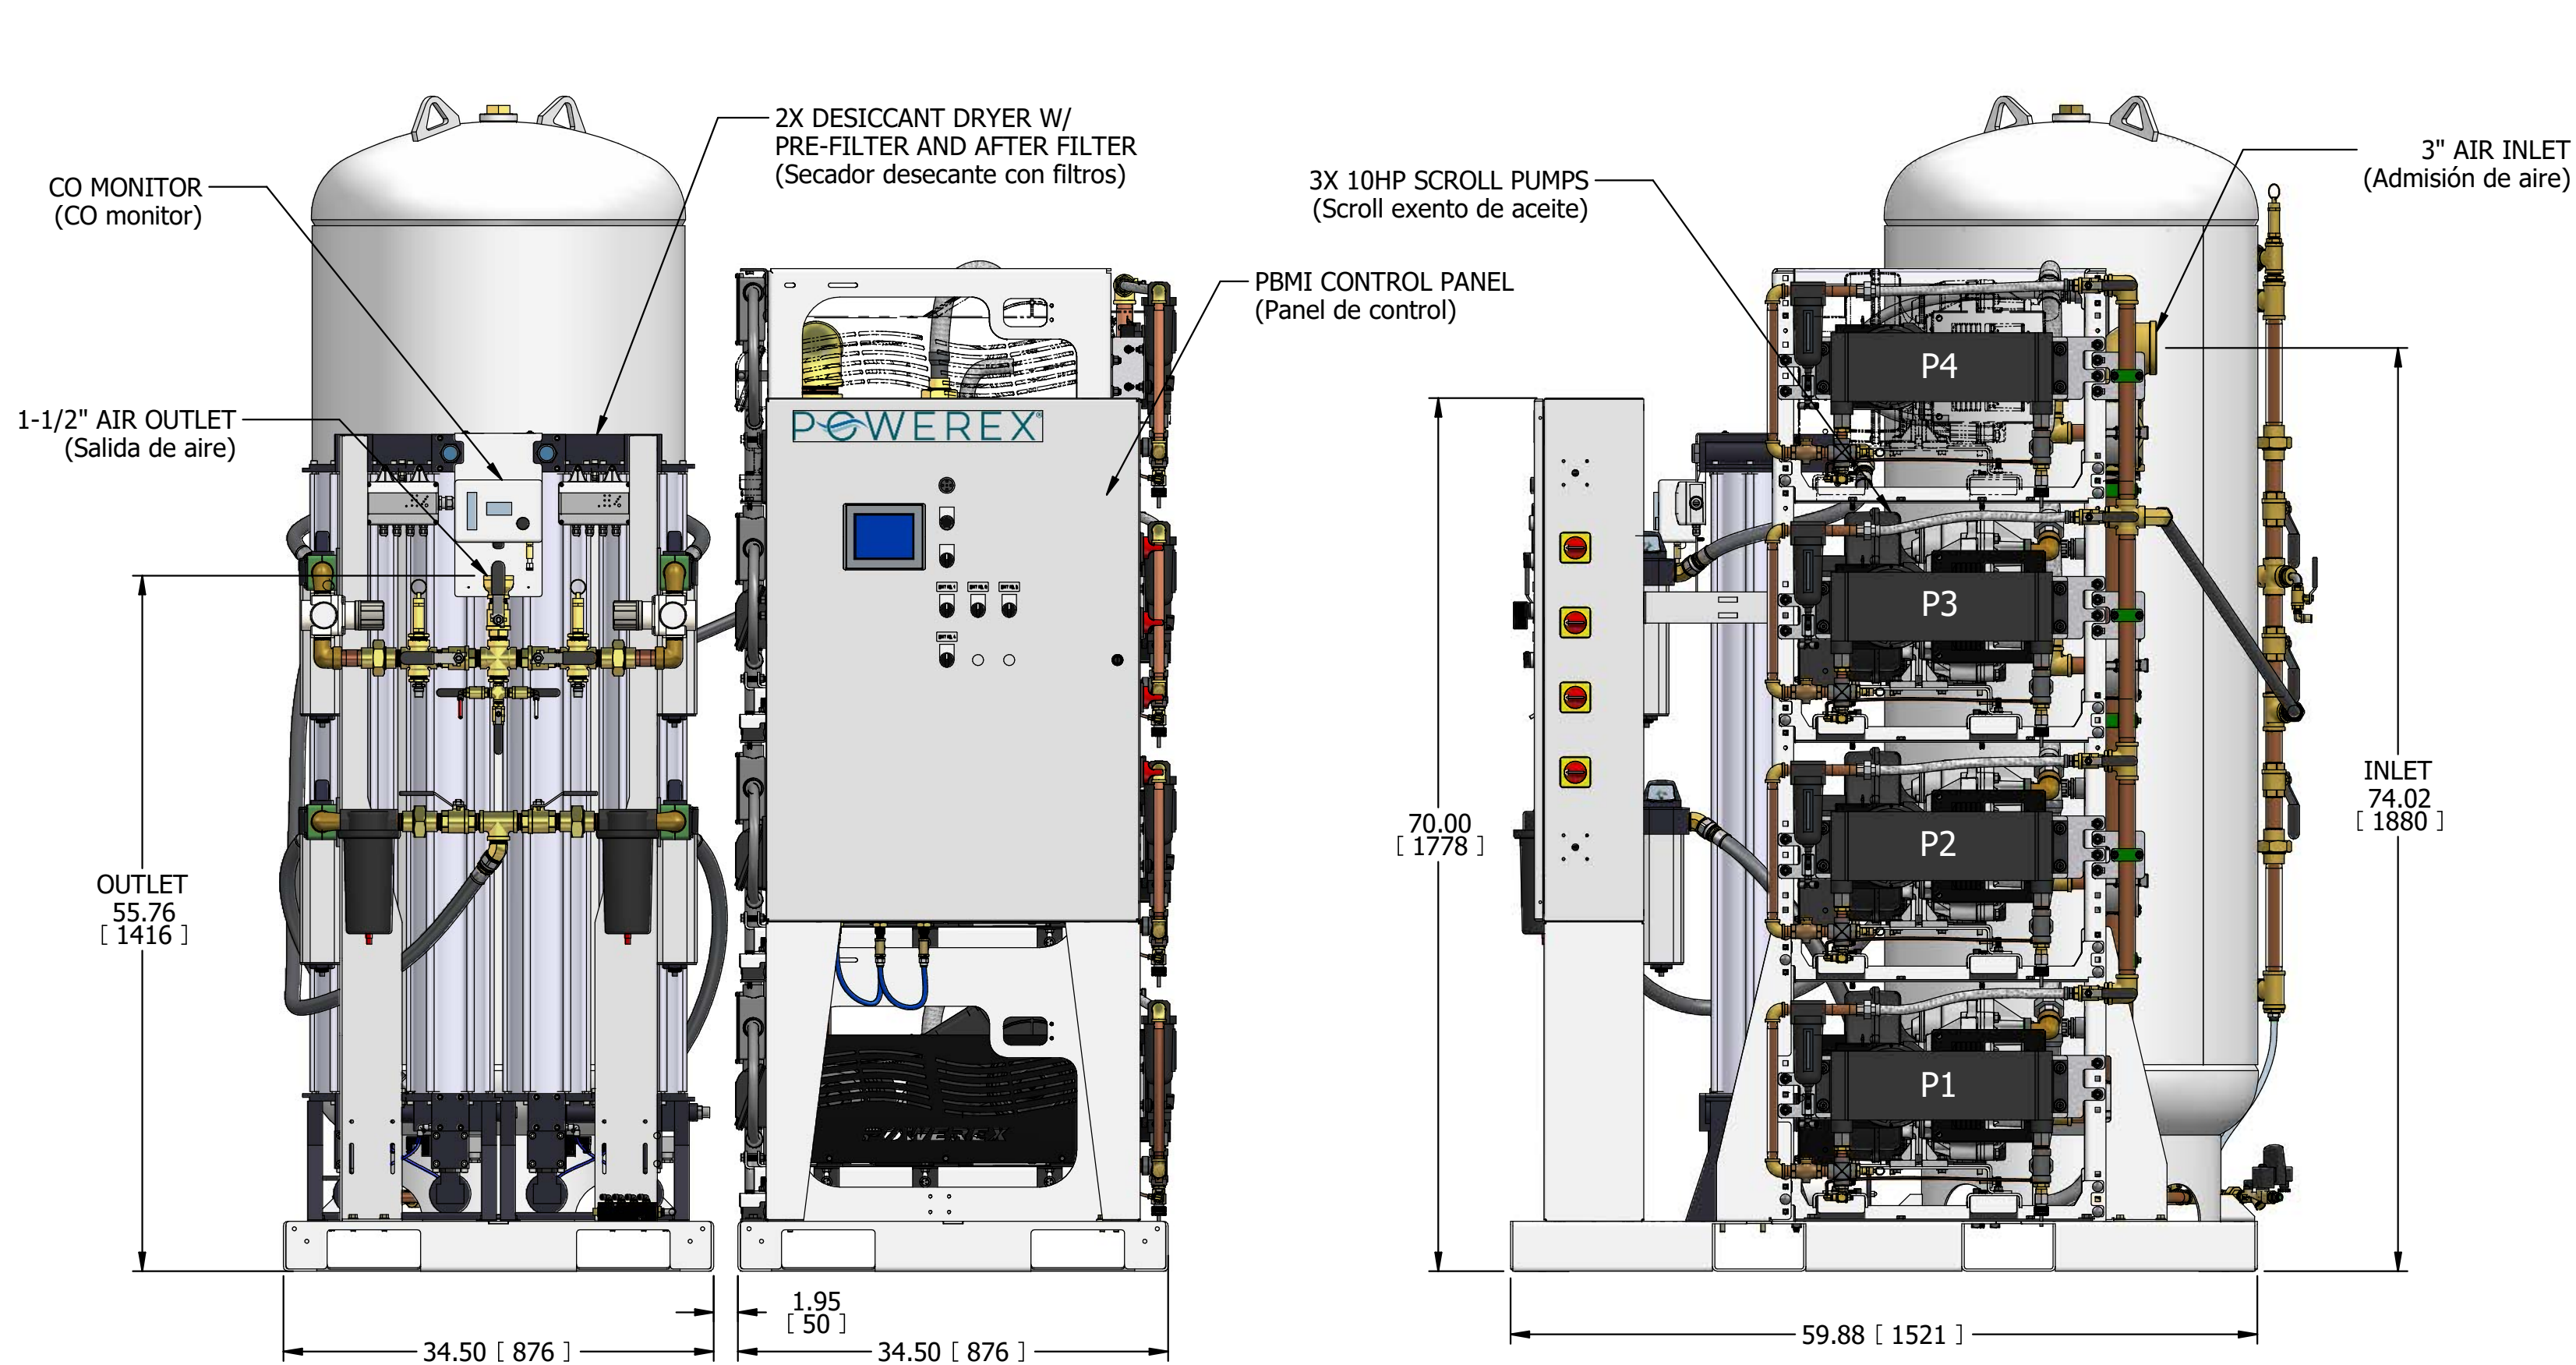
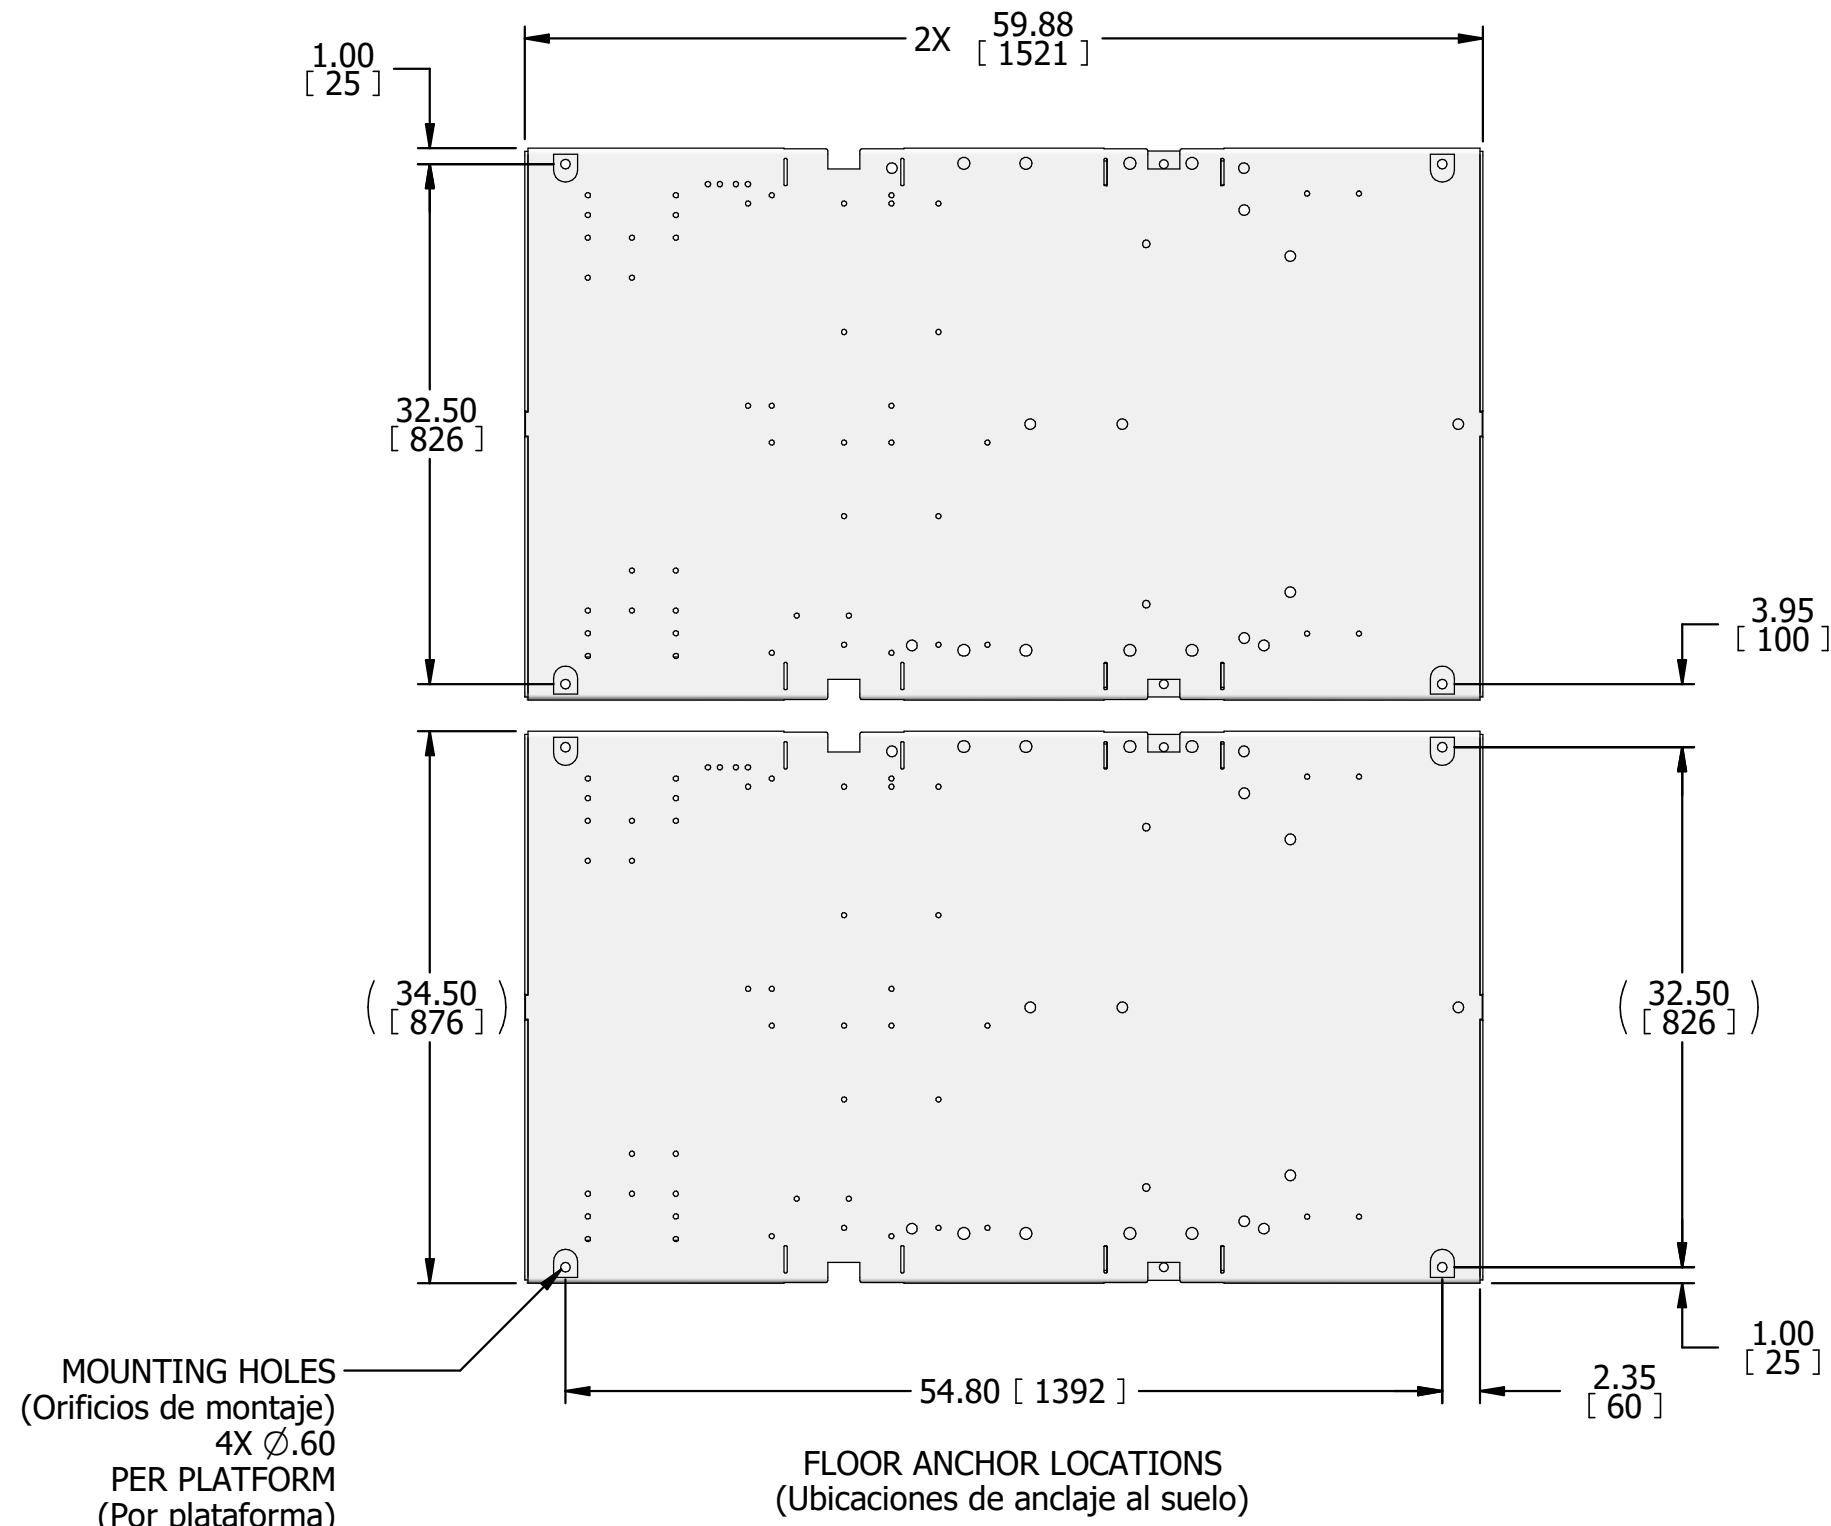




MST10C6xP5-EX4

10HP MED OPEN SCROLL TRIPLEX 240GAL EX4 DUPLEX DESICCANT

REVISION NOTES	
DESCRIPTION	ECN
PRODUCTION RELEASE	PXEC0318

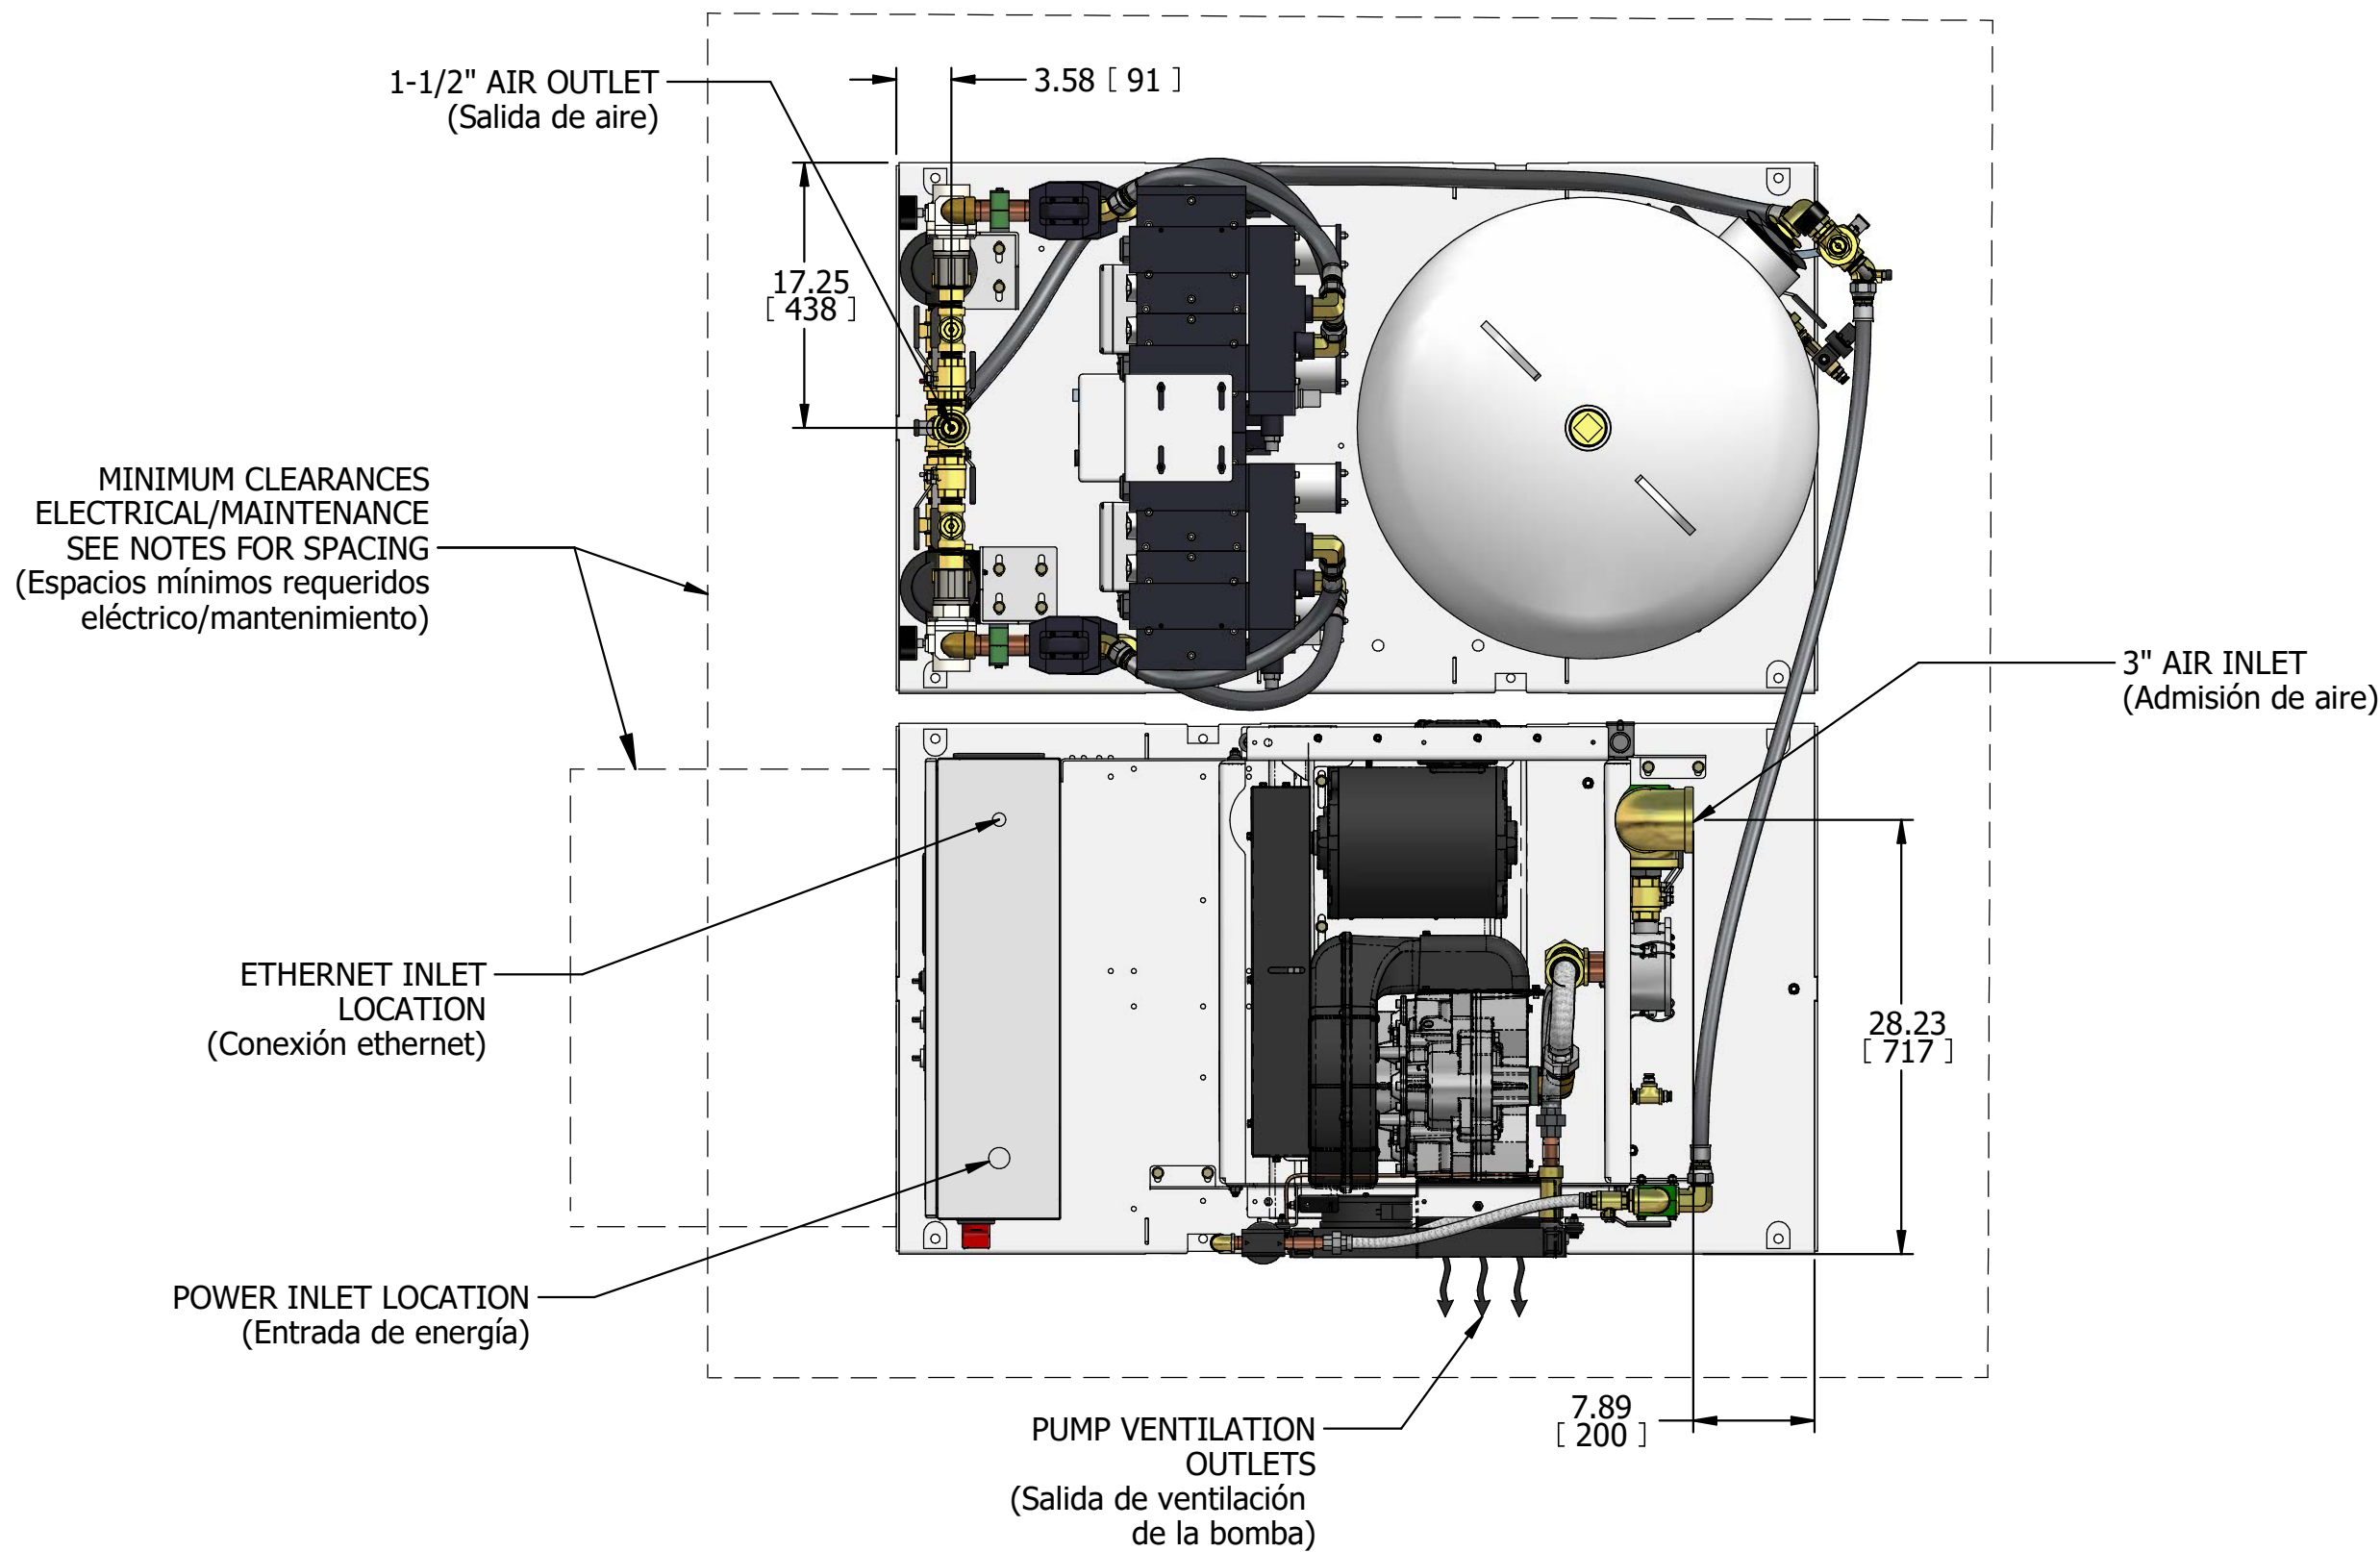


- NOTES:
1. APPROXIMATE WEIGHT: 3067 LBS
 2. A MINIMUM OF 24" CLEARANCE IS RECOMMENDED AROUND THE ENTIRE UNIT. CLEARANCE FOR CONTROL PANEL SHALL BE IN ACCORDANCE WITH OSHA/NEC REQUIREMENTS.
 3. SYSTEM DESIGNED IN COMPLIANCE WITH U.S. NFPA '99, LATEST EDITION.
 4. INLET AND OUTLET FLEX HOSES ADD 12" TO CONNECTIONS
1. PESO APROXIMADO: 1391 kg
2. RECOMENDAMOS QUE EL ESPACIO LIBRE ALREDEDOR DEL SISTEMA DEBE SER COMO MÍNIMO 24" (600 mm). EL ESPACIO LIBRE PARA EL TABLERO DE CONTROL DEBERÁ ESTAR DE ACUERDO CON LOS REQUERIMIENTOS DE SEGURIDAD DE LA OSHA/NEC.
3. EL SISTEMA ESTÁ DISEÑADO DE ACUERDO CON LA ÚLTIMA EDICIÓN DE LA NFPA 99.
4. LAS MANGUERAS FLEXIBLES DE ENTRADA Y SALIDA AÑADEN 12" A LAS CONEXIONES

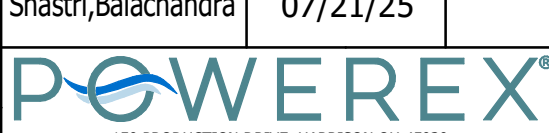SYMBOL LEGEND				DRAWINGS TO CONFORM TO CURRENT REVISION OF THE FOLLOWING ANSI STANDARDS: Y14.3 MULTI AND SECTIONAL VIEW DWGS Y14.5 DIMENSIONING AND TOLERANCING	
TOLERANCES, UNLESS OTHERWISE SPECIFIED		SOLID EDGE DRAWING		DO NOT SCALE DRAWING FOR DIMENSIONS	
0.XX ± .05		INCH [mm]		SHEET 1 OF 2	
0.XXX ± .005					
± .1					
CONFIDENTIAL DISCLOSURE This drawing is the property of POWEREX INC. of HARRISON HOLDINGS, INC. and is subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.		AUTHOR		REVISION DATE	
		Shastri, Balachandra		07/21/25	
				APPROVALS ON FILE IN PLM	
ITEM ID: 761026					
MATERIAL: ---					
		150 PRODUCTION DRIVE, HARRISON OH 45030 (888) 769-7979			
DESCRIPTION 10HP MED OPEN SCROLL TRIPLEX 240GAL EX4 DUPLEX DESICCANT		DRAWING NUMBER MST10C6xP5-EX4		REVISION B	
				SIZE D	

MST10C6xP5-EX4

10HP MED OPEN SCROLL TRIPLEX 240GAL EX4 DUPLEX DESICCANT

REVISION NOTES	
DESCRIPTION	ECN
PRODUCTION RELEASE	PXEC0318

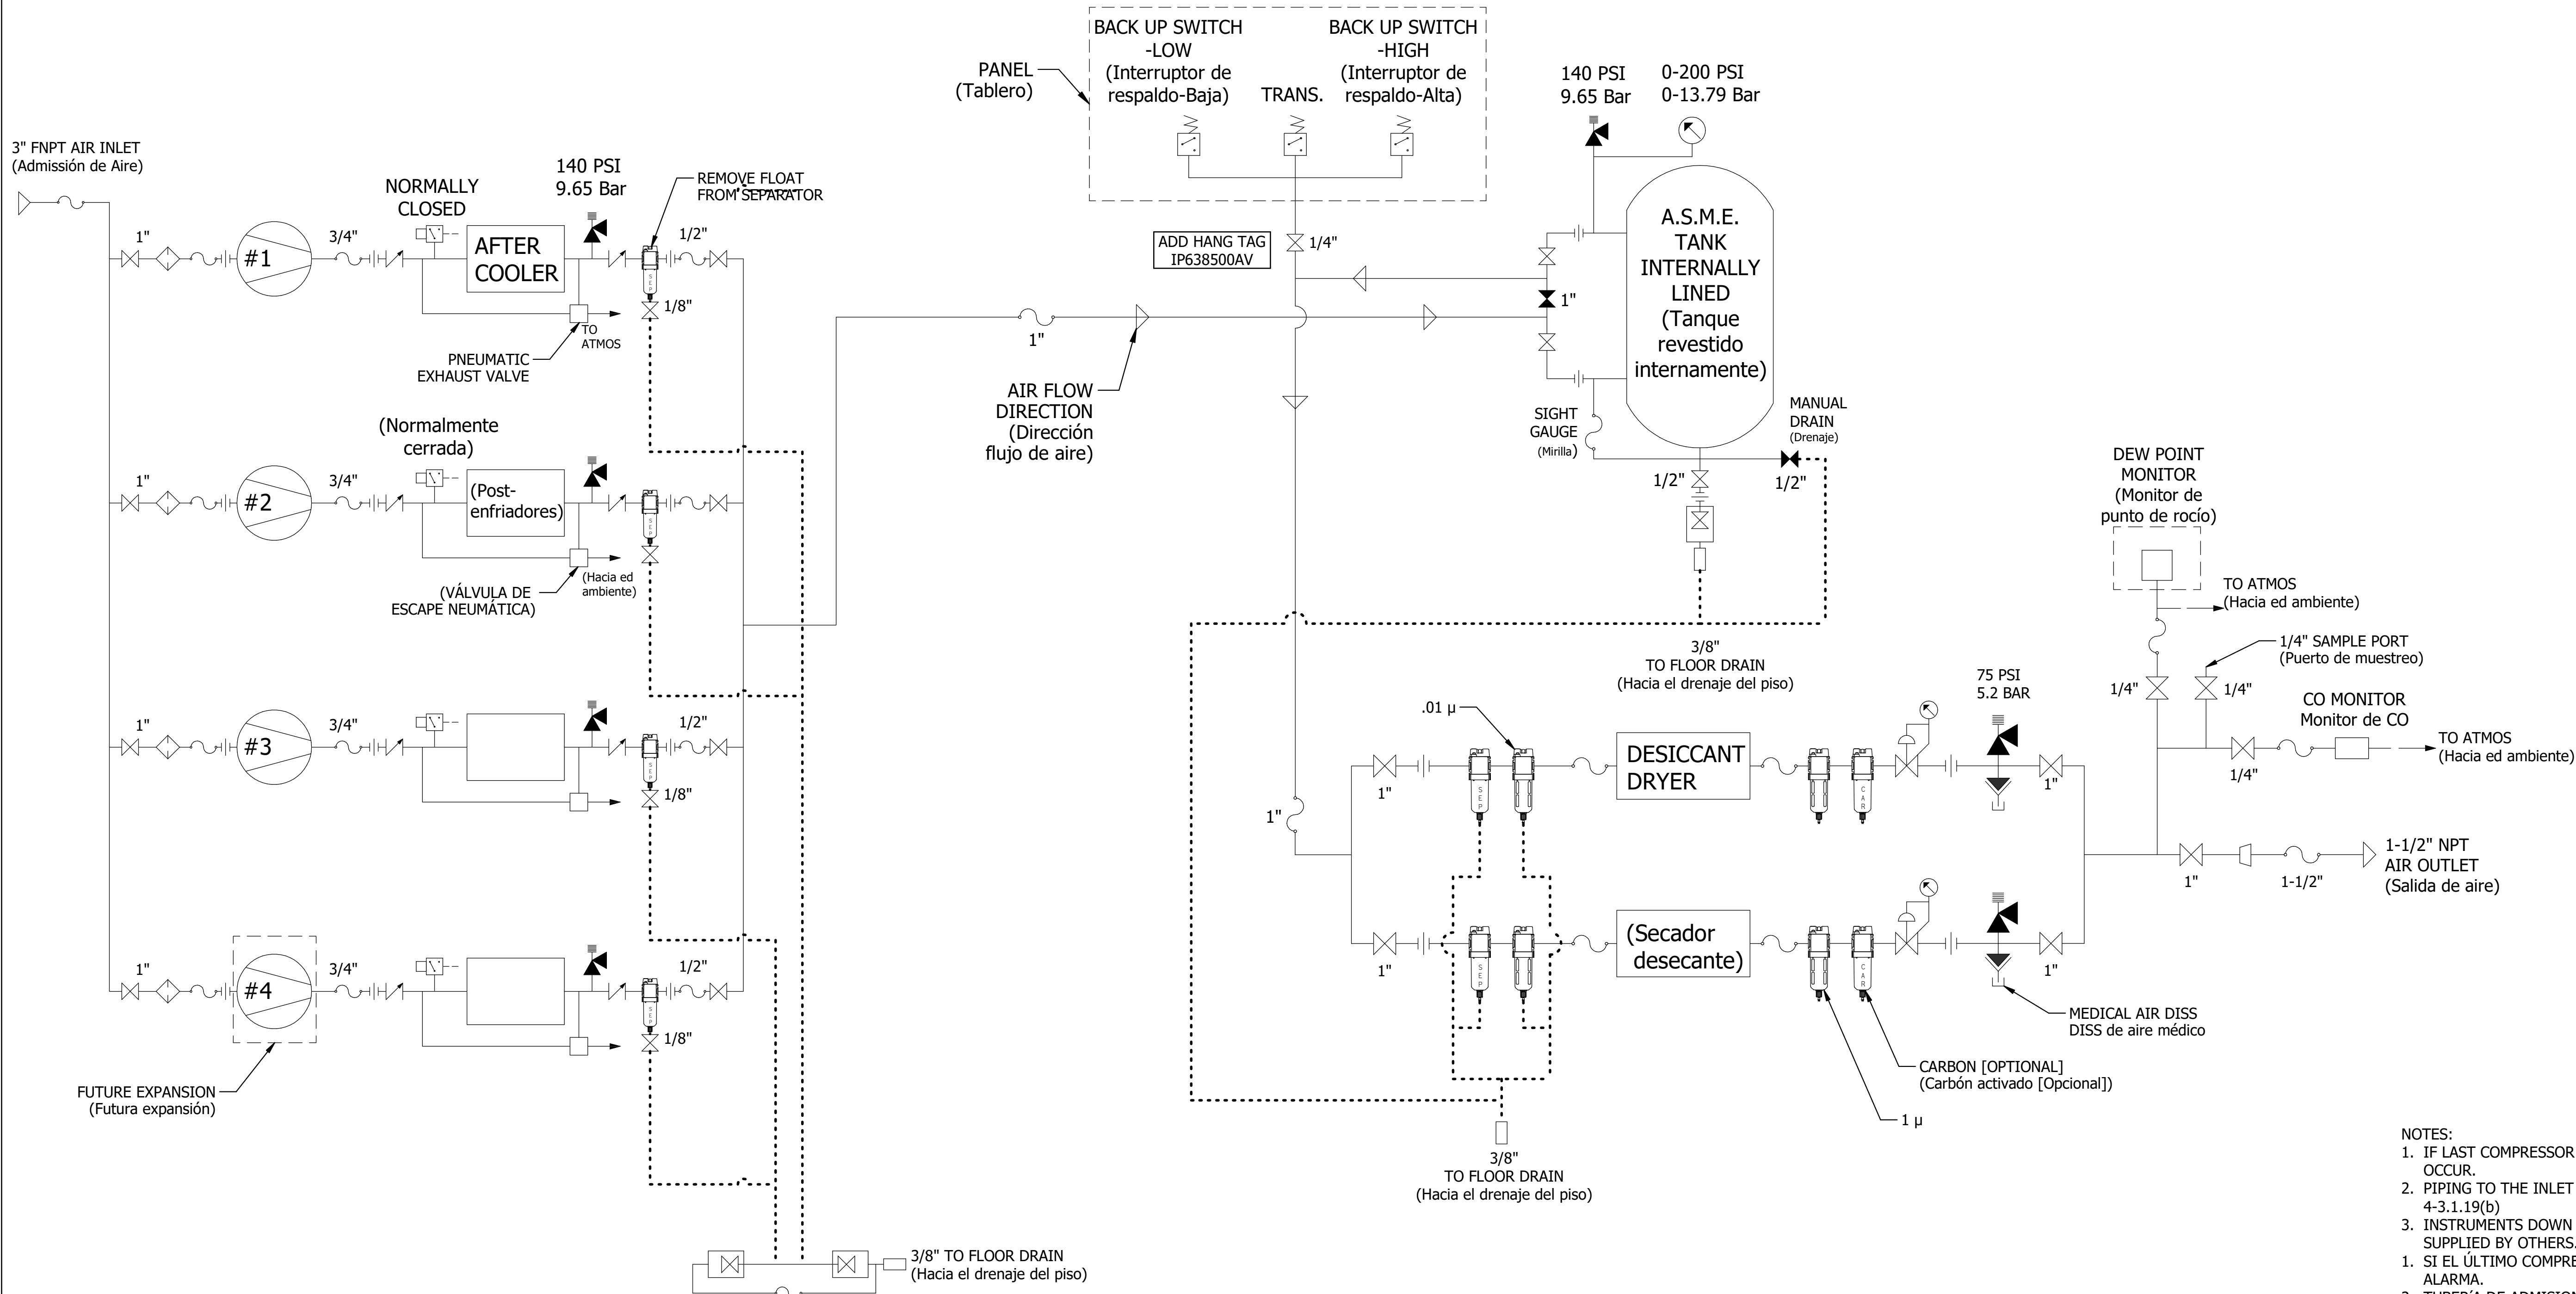

- NOTES:
- IF LAST COMPRESSOR PLEX IS ENERGIZED ALARM WILL OCCUR.
 - PIPING TO THE INLET BY OTHERS AND TO BE PER NFPA99 4-3.1.19(b)
 - INSTRUMENTS DOWN STREAM OF SOURCE VALVE TO BE SUPPLIED BY OTHERS.
 - SI EL ÚLTIMO COMPRESOR SE ACTIVA, SE PRODUCIRÁ UNA ALARMA.
 - TUBERÍA DE ADMISION POR OTROS Y CUMPLIR CON LA NFPA 99 4-3.1.19 (b).
 - ACCESORIOS AGUAS-ABAJO DE LA VALVULA DE CORTE DE SUMINISTRO SERAN INSTALADOS POR OTROS.

SYMBOL LEGEND		DRAWINGS TO CONFORM TO CURRENT REVISION OF THE FOLLOWING AISC STANDARDS:	
		Y14.3 MULTI AND SECTIONAL VIEW DWGS	
		Y14.5 DIMENSIONING AND TOLERANCING	
TOLERANCES, UNLESS OTHERWISE SPECIFIED	SOLID EDGE DRAWING	DO NOT SCALE DRAWING FOR DIMENSIONS	
0.XX ± .05			
0.XXX ± .005	INCH [mm]		
± .1			
CONFIDENTIAL DISCLOSURE This drawing is the property of POWEREX INC. of HARRISON HOLDINGS, INC. and is subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.			
DRAWING NUMBER		AUTHOR	REVISION DATE
761026		Shastri, Balachandra	07/21/25
MATERIAL			
150 PRODUCTION DRIVE, HARRISON OH 45030 (888) 766-7979			
DESCRIPTION		DRAWING NUMBER	REVISION
10HP MED OPEN SCROLL TRIPLEX 240GAL EX4 DUPLEX DESICCANT		MST10C6xP5-EX4	B
		SIZE	D