
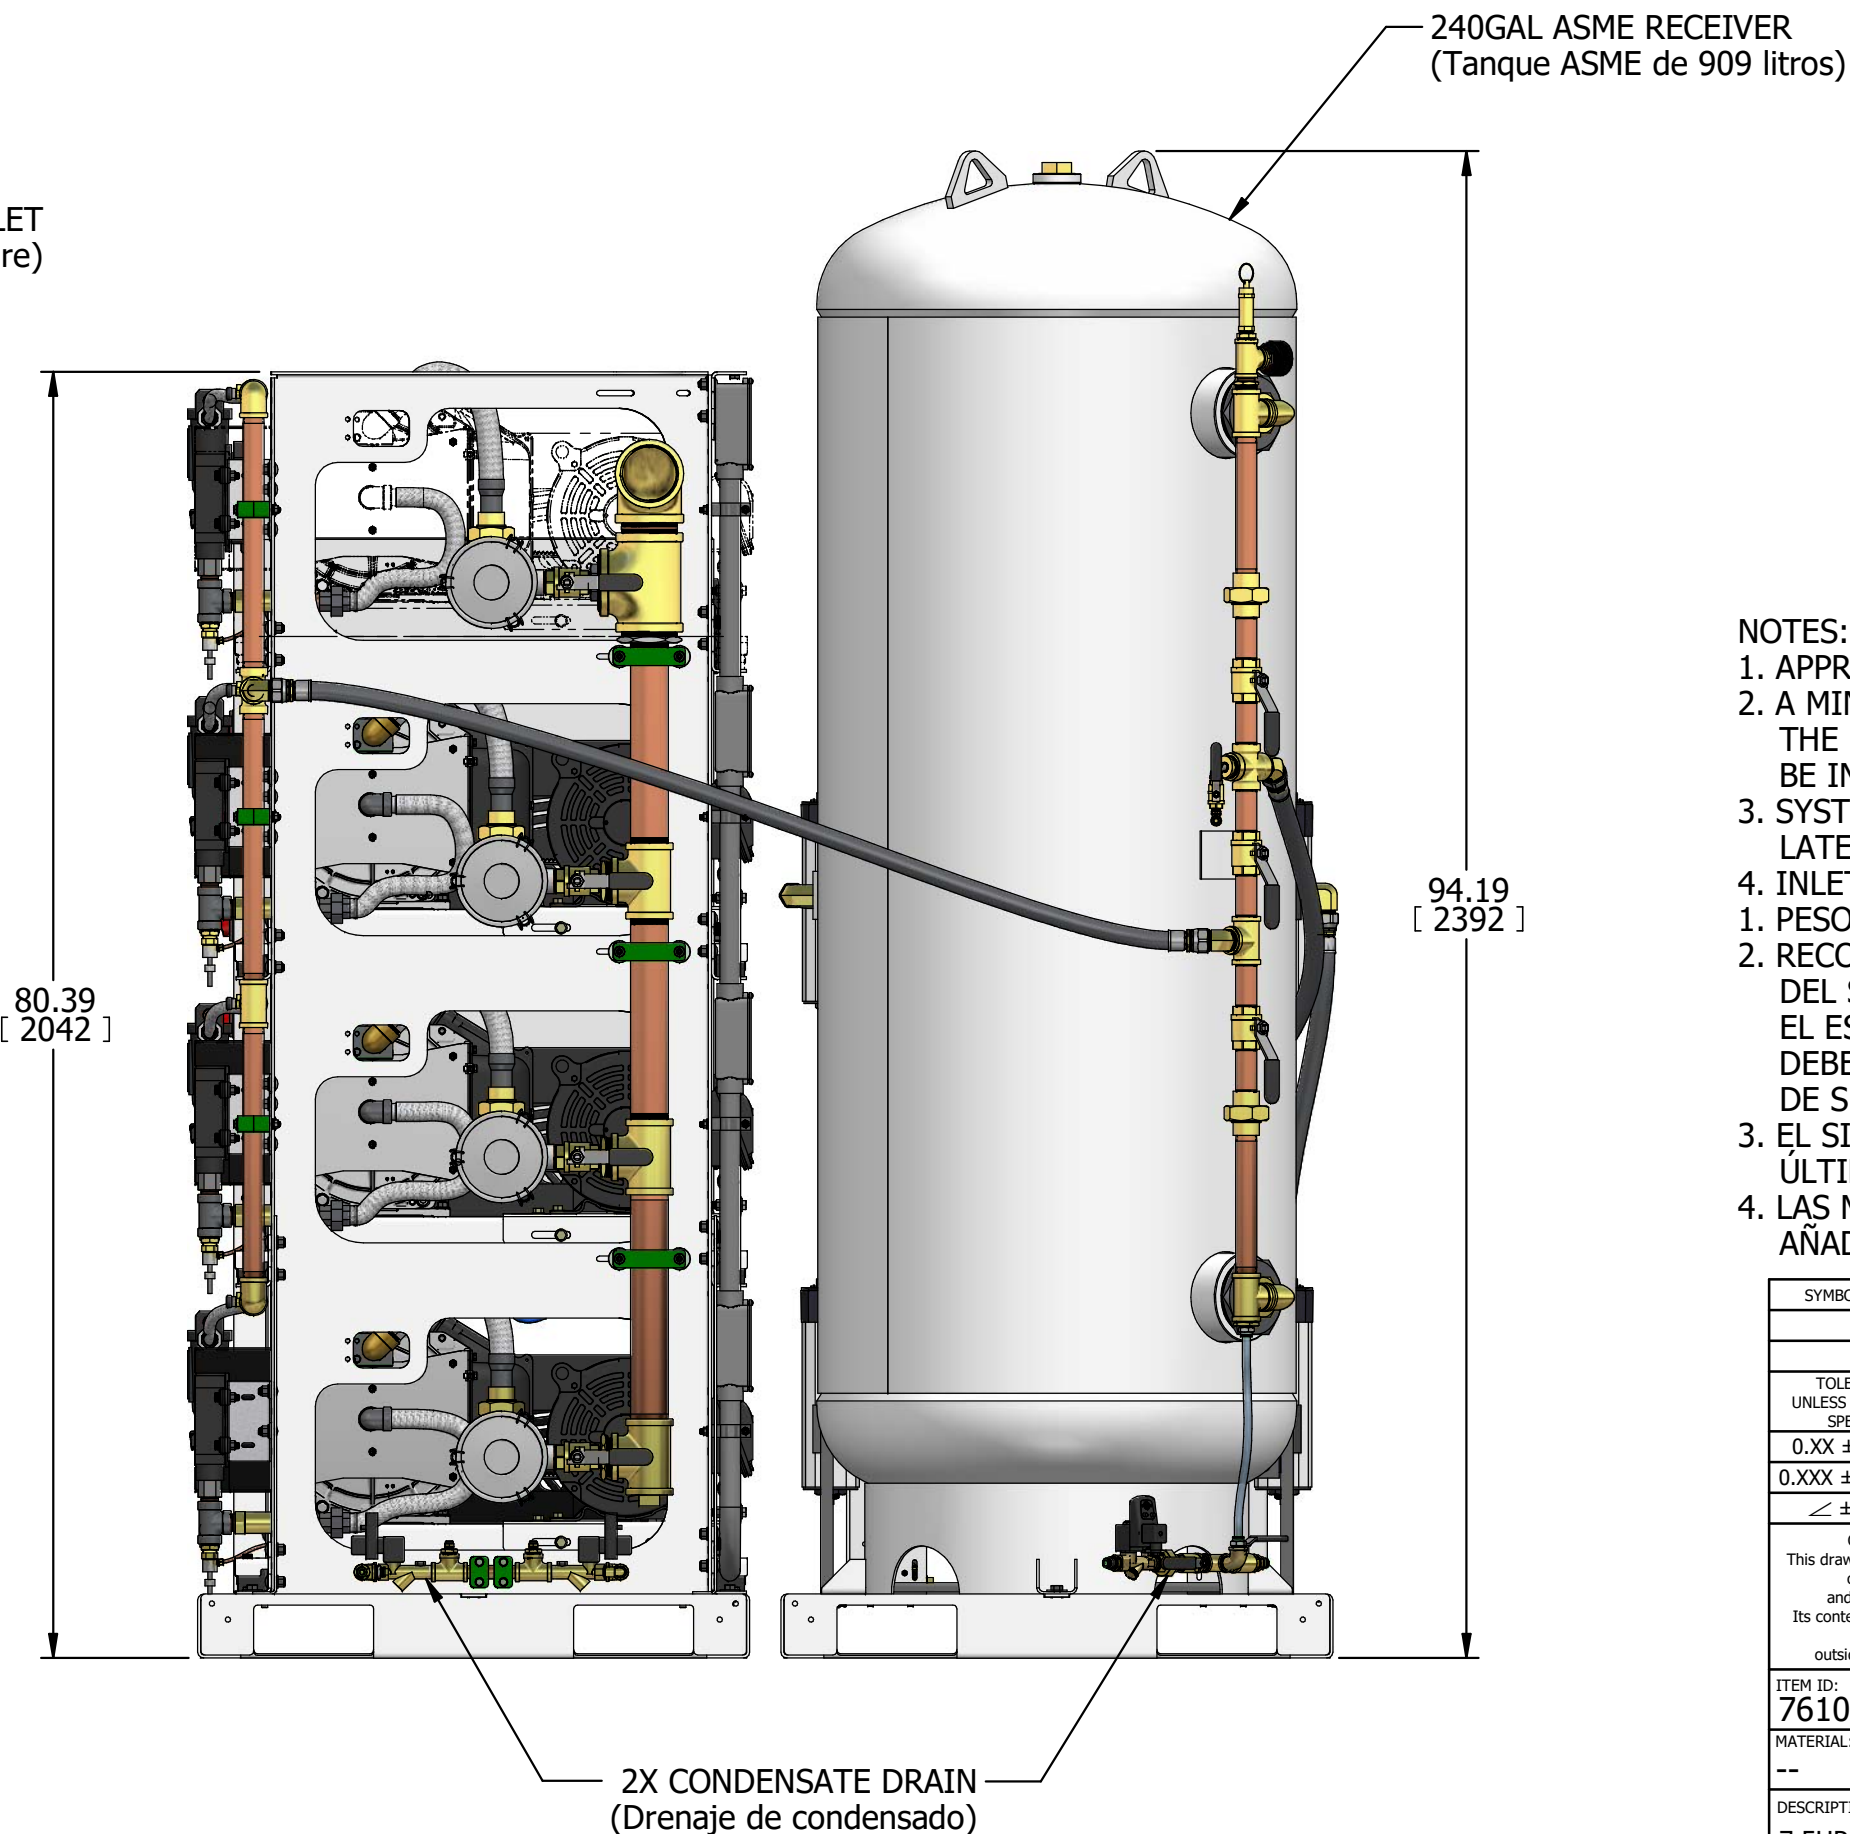
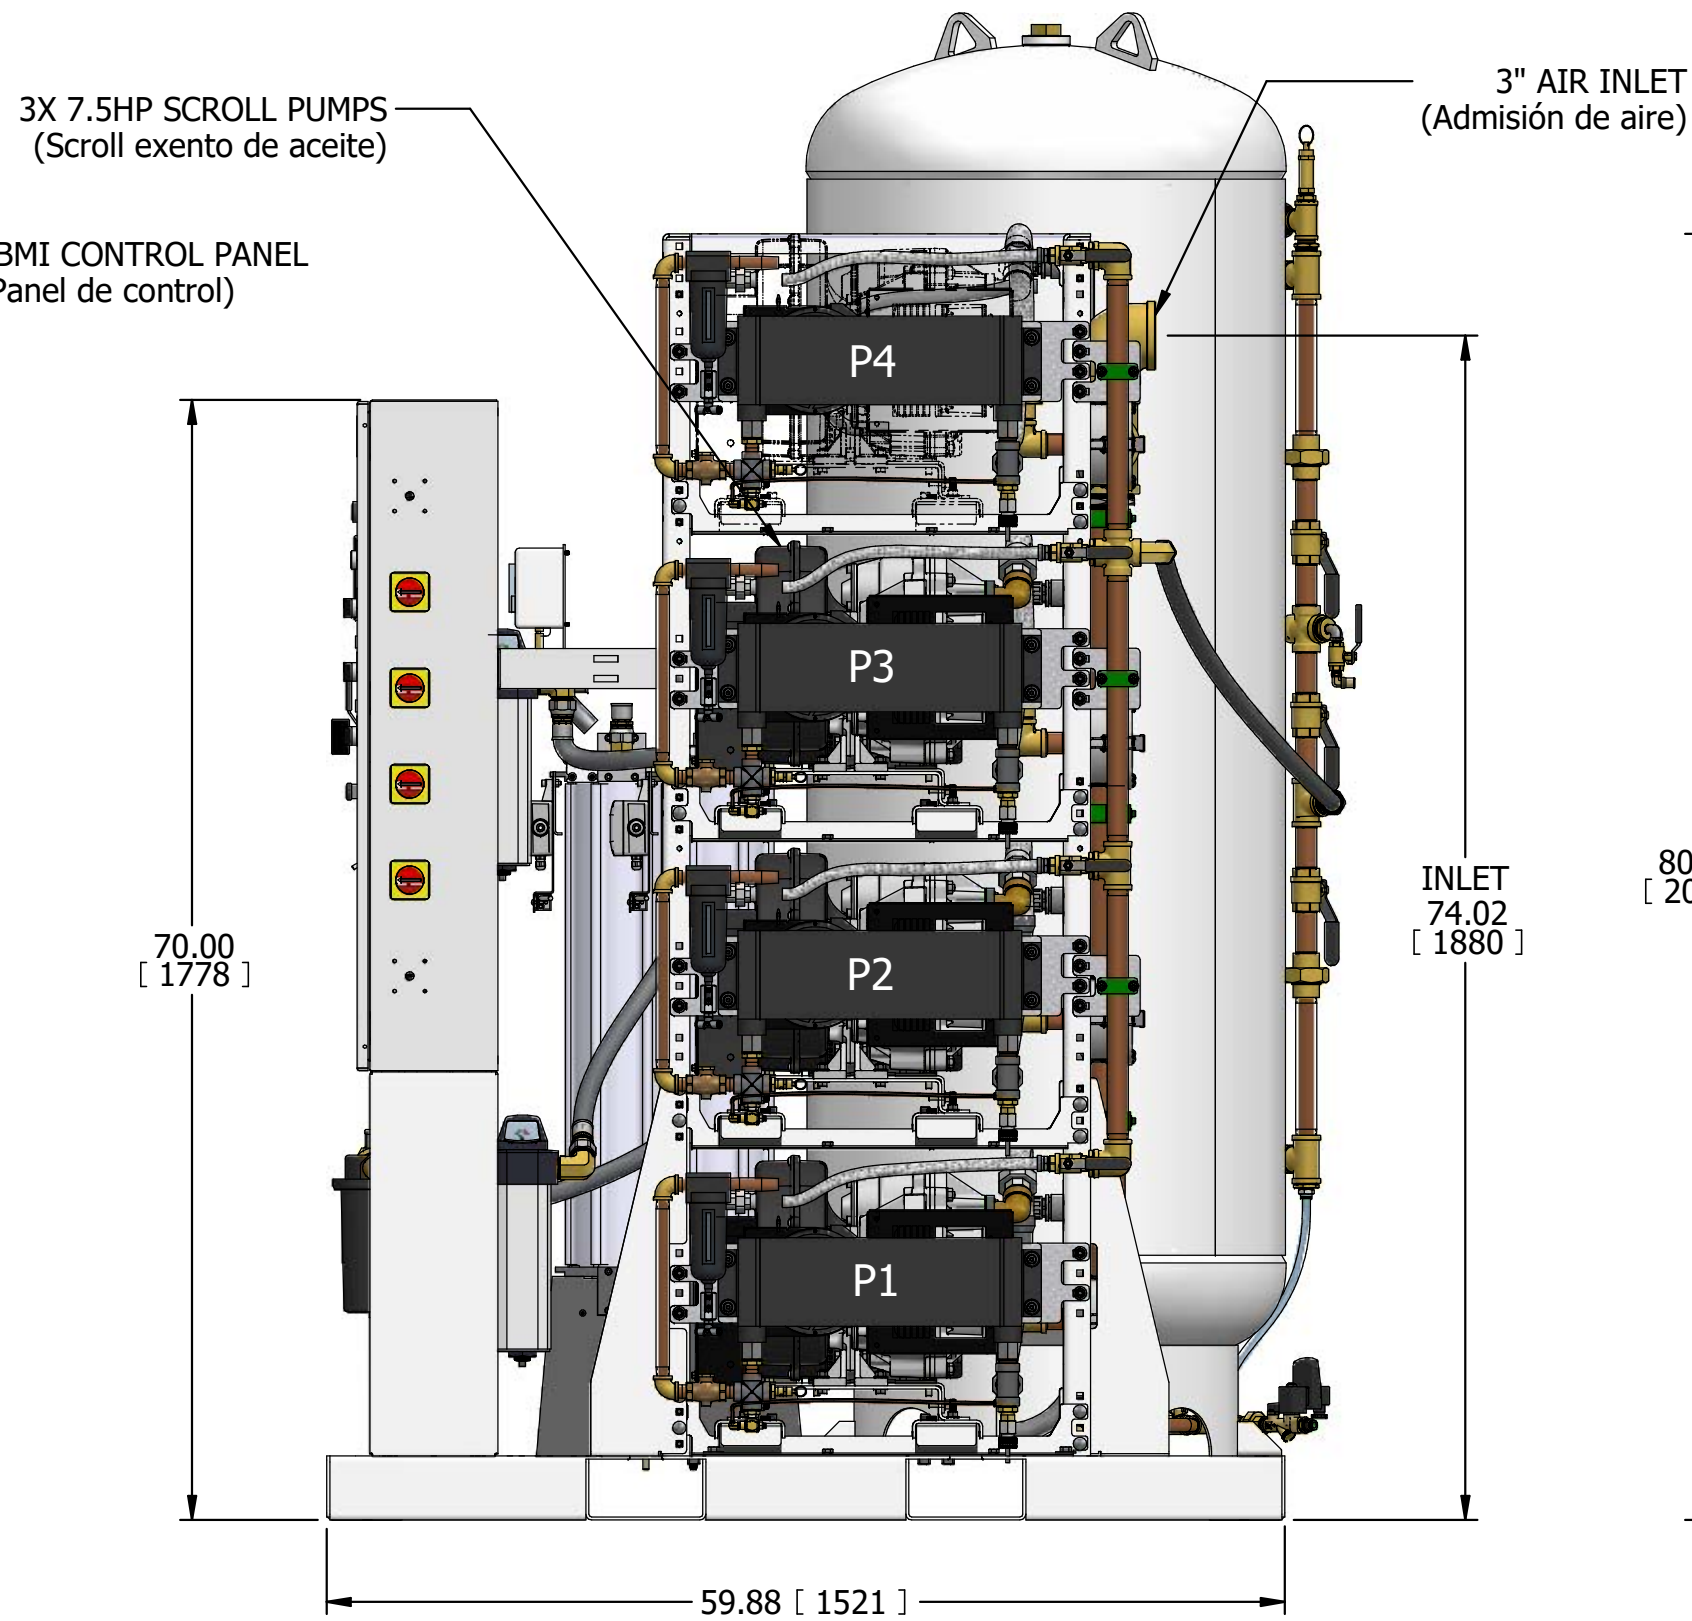
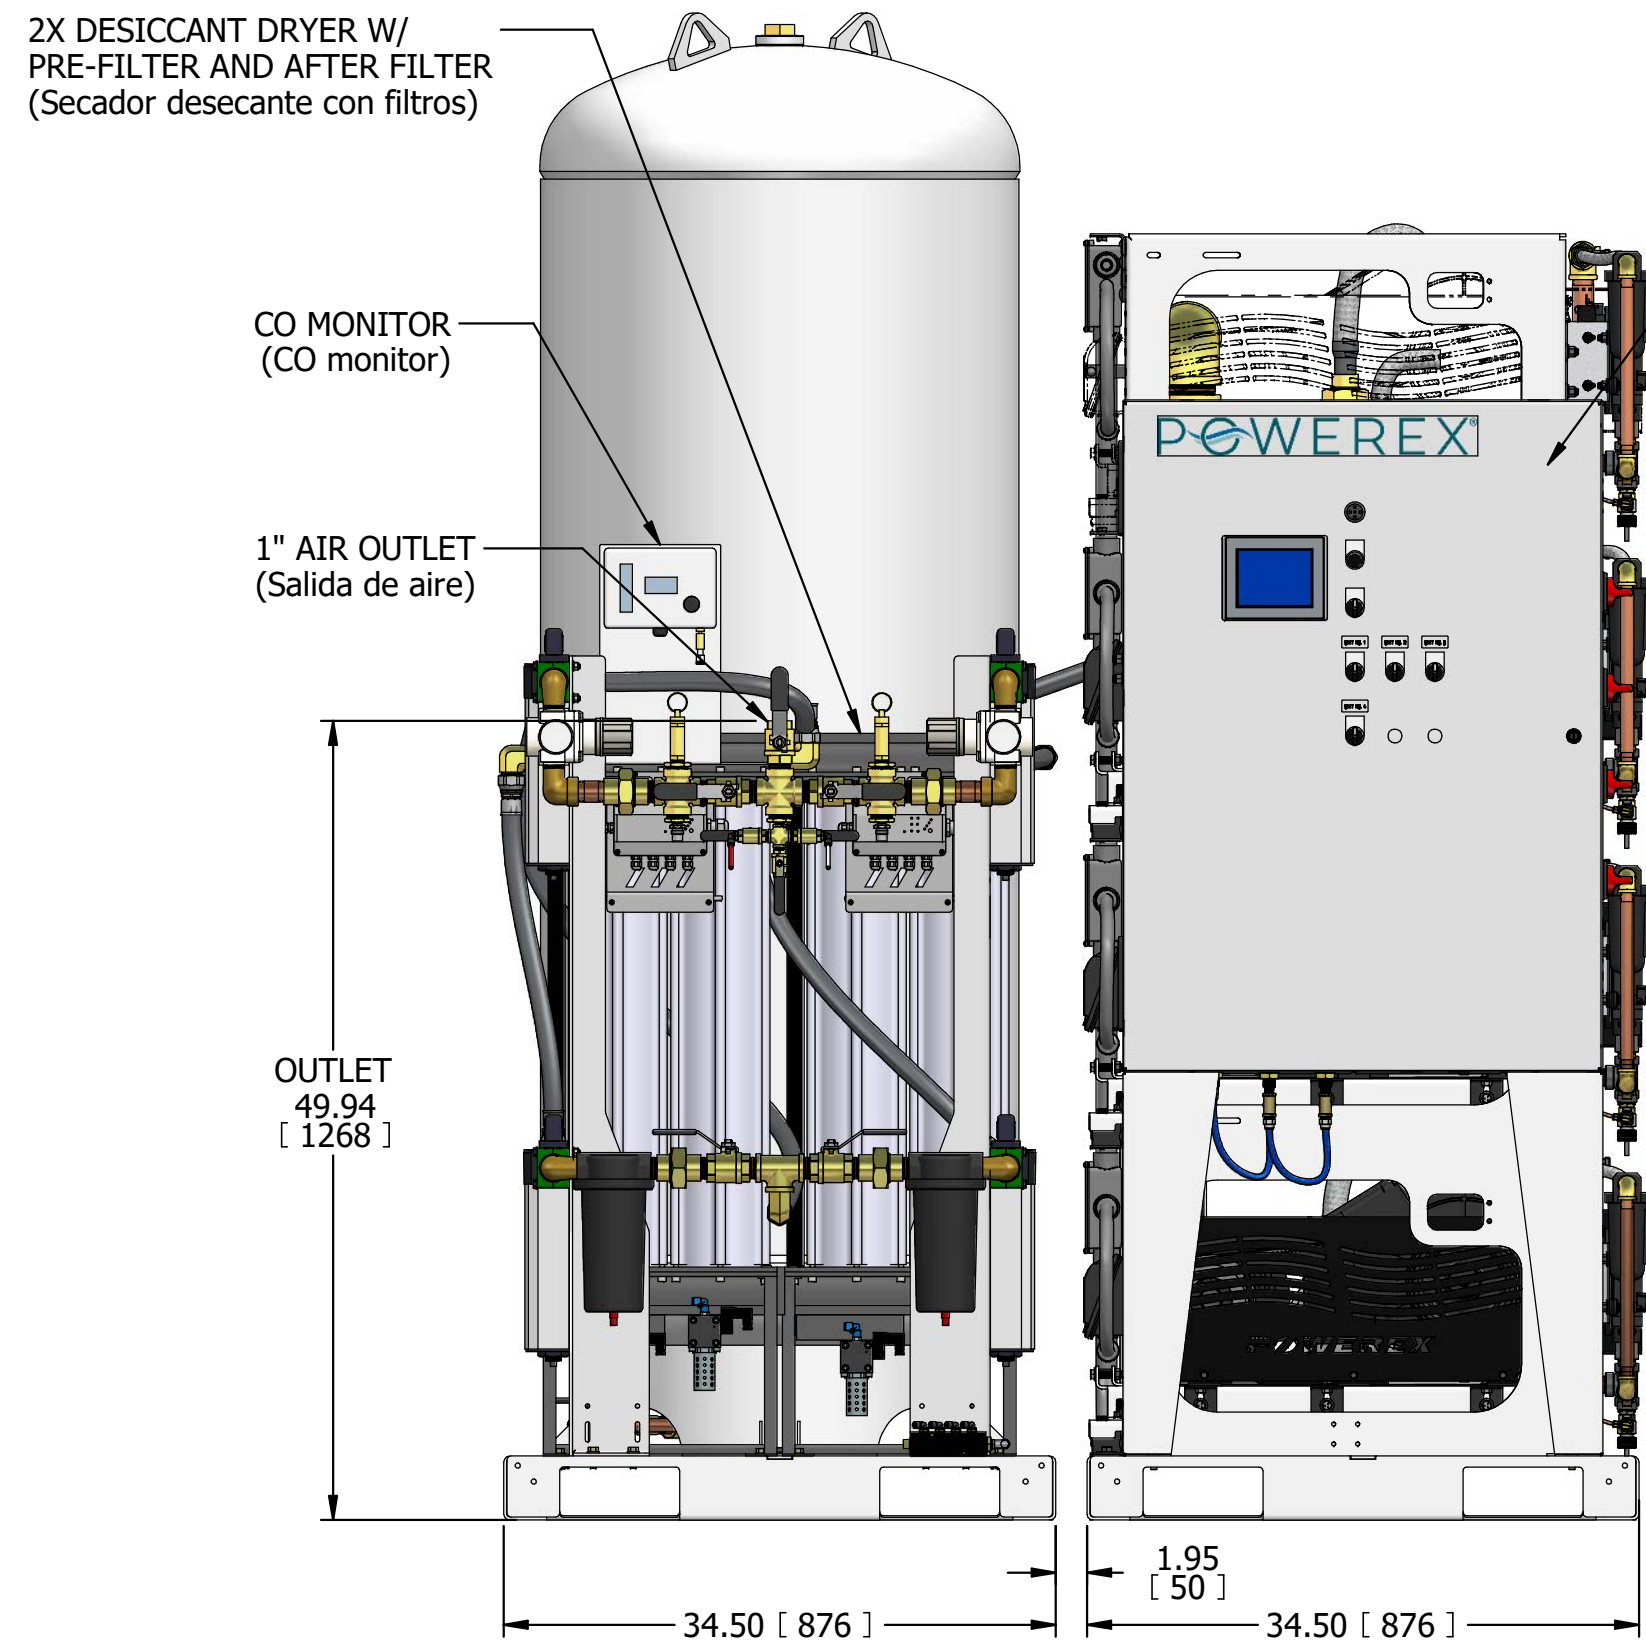
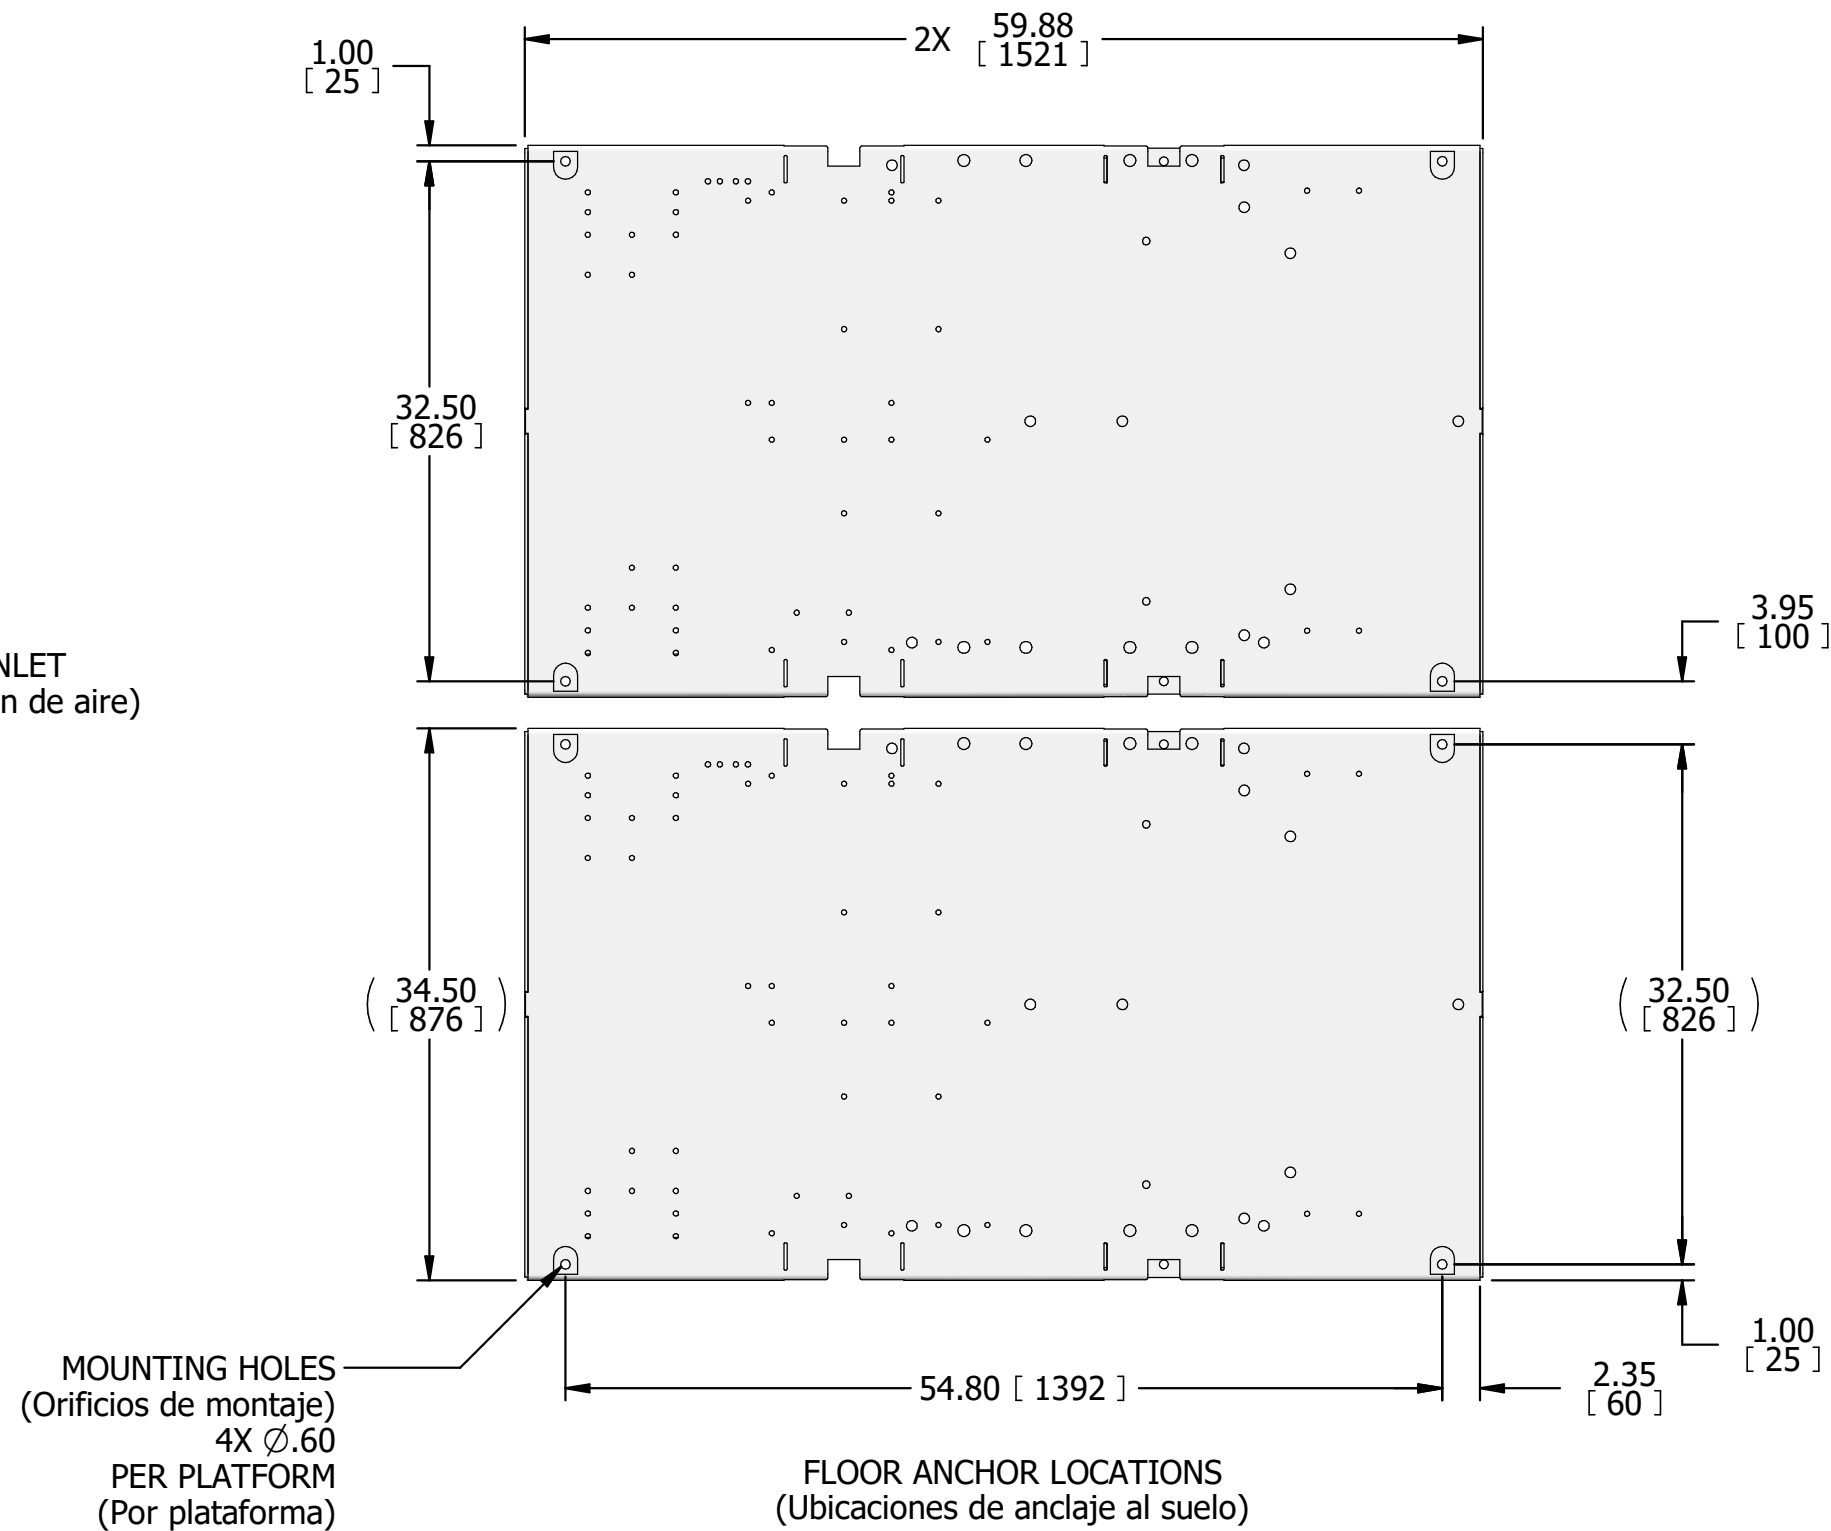


MST07C6xP5-EX4

7.5HP MED OPEN SCROLL TRIPLEX 240GAL EX4 DUPLEX DESICCANT

REVISION NOTES	
DESCRIPTION	ECN
PRODUCTION RELEASE	PXEC0318

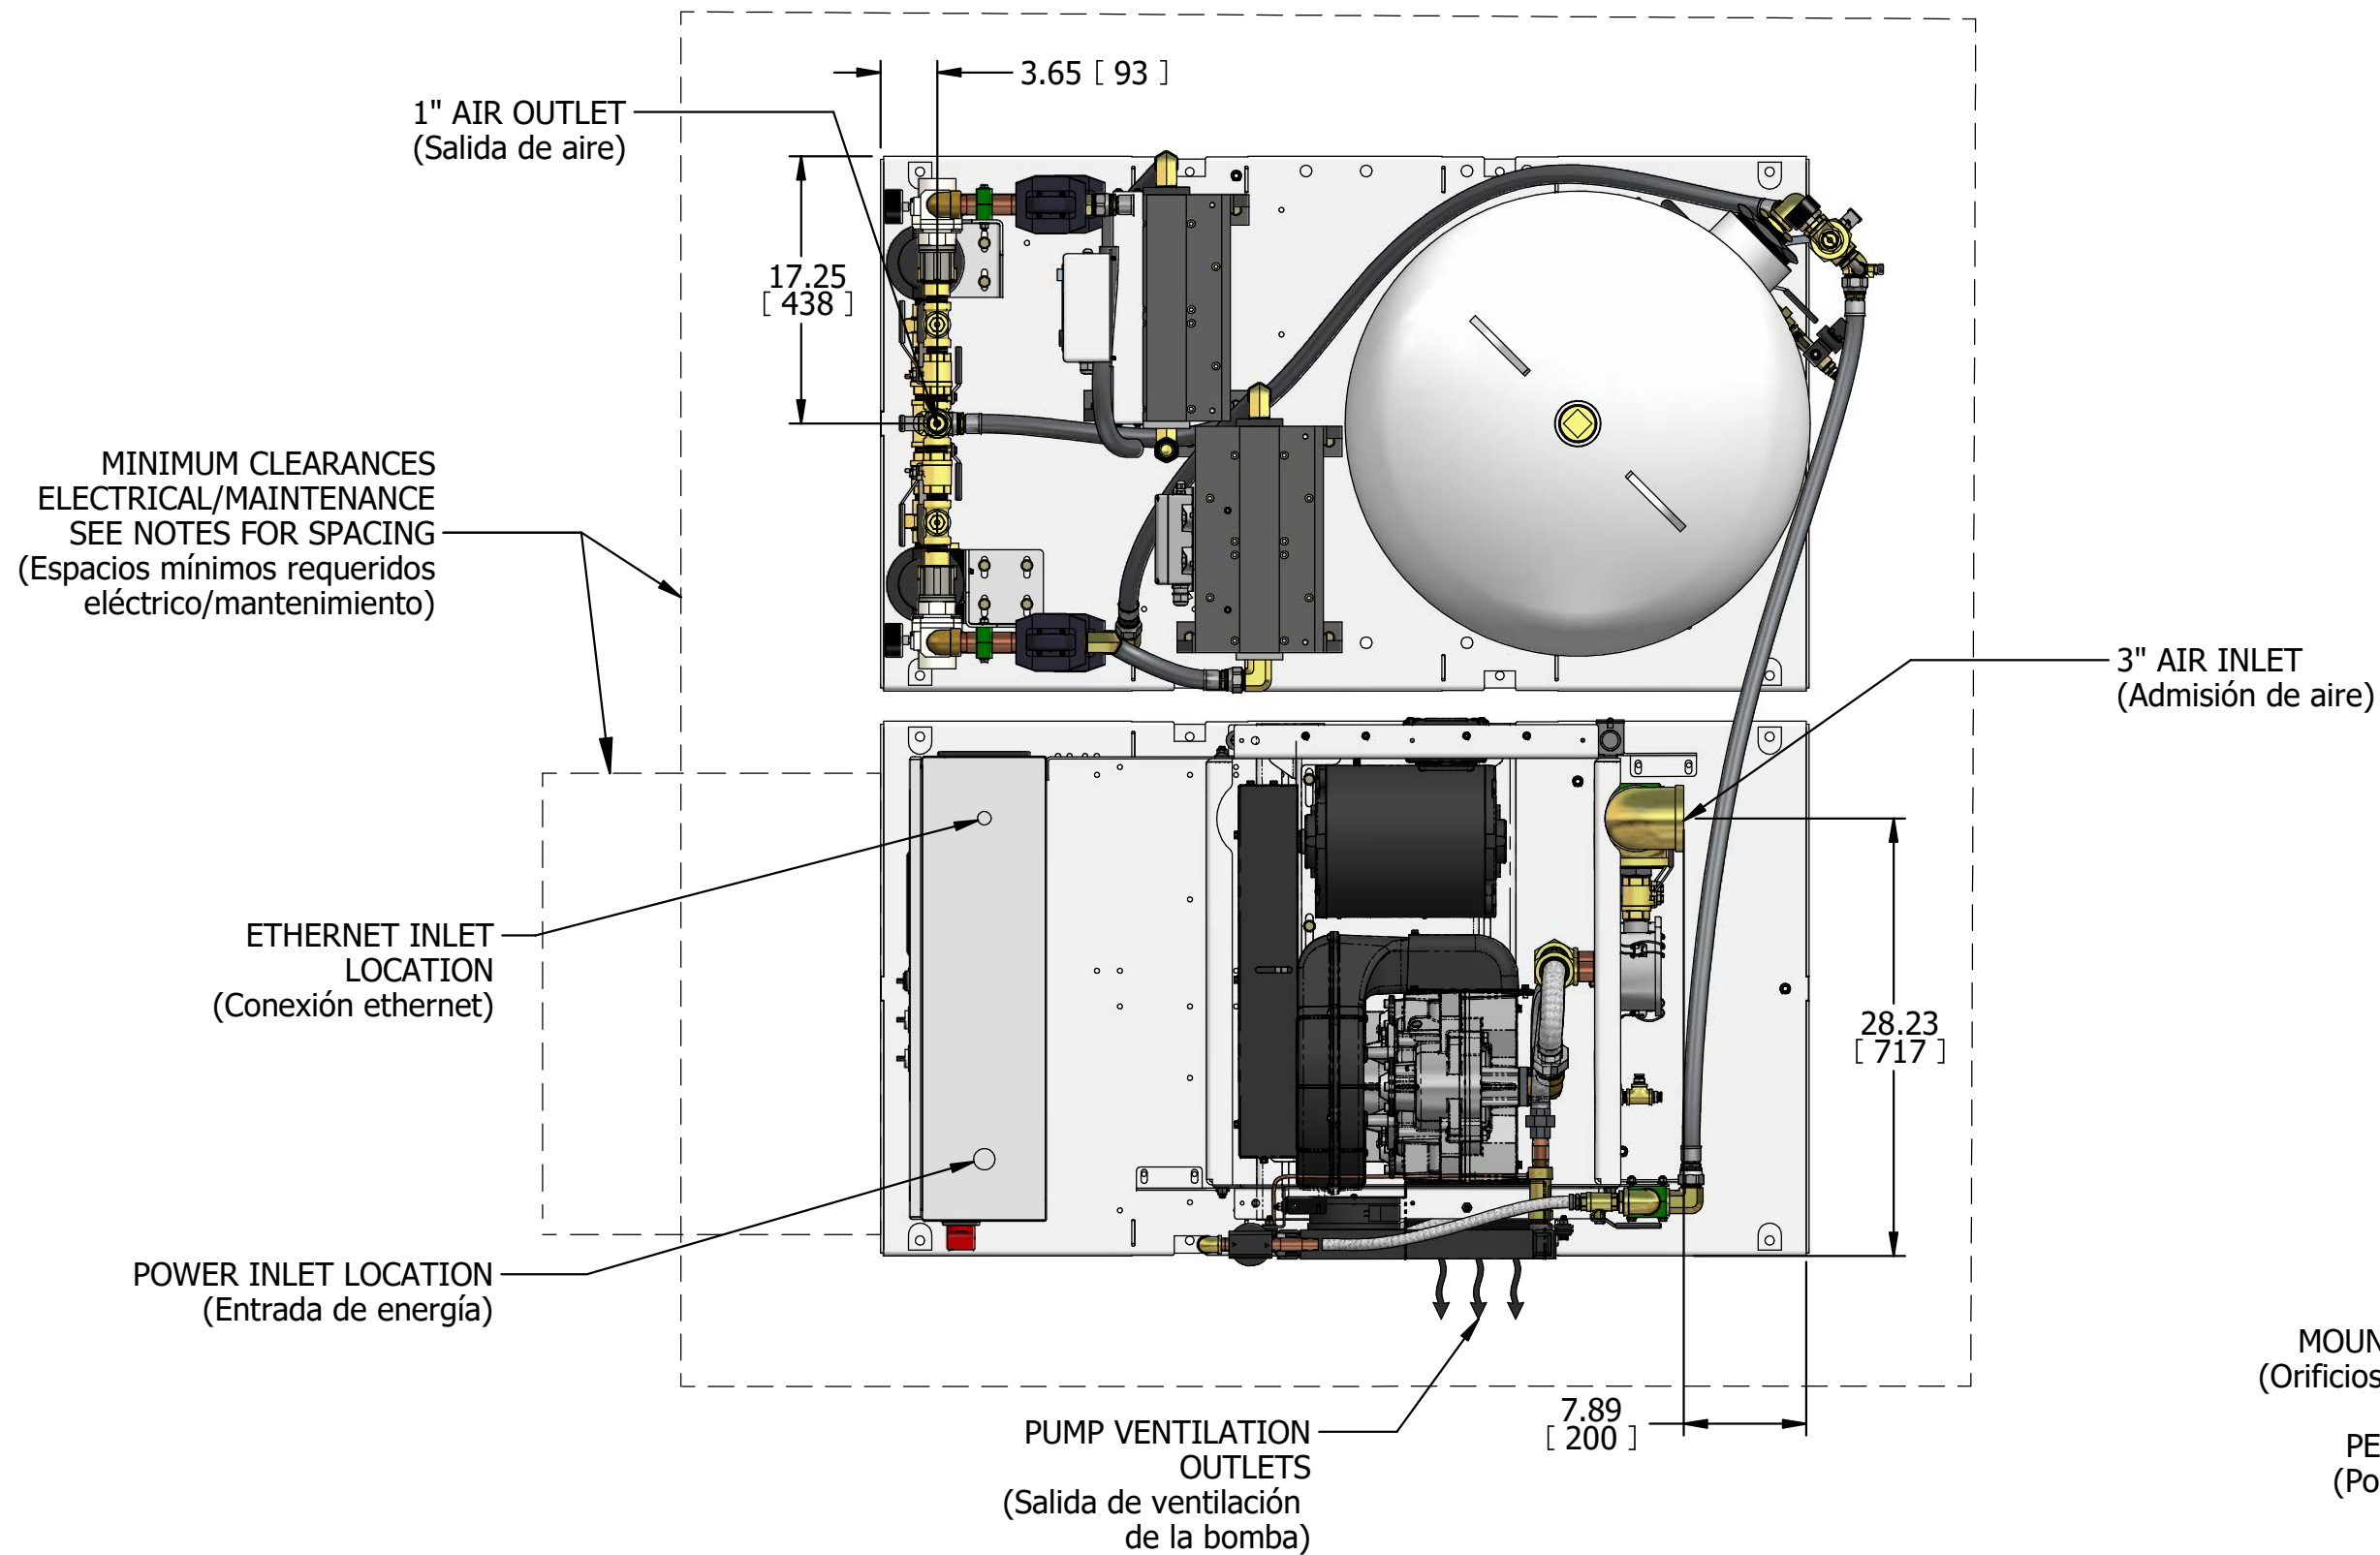


- NOTES:
1. APPROXIMATE WEIGHT: 2793 LBS
 2. A MINIMUM OF 24" CLEARANCE IS RECOMMENDED AROUND THE ENTIRE UNIT. CLEARANCE FOR CONTROL PANEL SHALL BE IN ACCORDANCE WITH OSHA/NEC REQUIREMENTS.
 3. SYSTEM DESIGNED IN COMPLIANCE WITH U.S. NFPA '99, LATEST EDITION.
 4. INLET AND OUTLET FLEX HOSES ADD 12" TO CONNECTIONS
 1. PESO APROXIMADO: 1267 kg
 2. RECOMENDAMOS QUE EL ESPACIO LIBRE ALREDEDOR DEL SISTEMA DEBE SER COMO MÍNIMO 24" (600 mm). EL ESPACIO LIBRE PARA EL TABLERO DE CONTROL DEBERÁ ESTAR DE ACUERDO CON LOS REQUERIMIENTOS DE SEGURIDAD DE LA OSHA/NEC.
 3. EL SISTEMA ESTÁ DISEÑADO DE ACUERDO CON LA ÚLTIMA EDICIÓN DE LA NFPA 99.
 4. LAS MANGUERAS FLEXIBLES DE ENTRADA Y SALIDA AÑADEN 12" A LAS CONEXIONES

SYMBOL LEGEND		DRAWINGS TO CONFORM TO CURRENT REVISION OF THE FOLLOWING ANSI STANDARDS: Y14.36 SECTIONAL VIEW DWGS Y14.5 DIMENSIONING AND TOLERANCING					
							
TOLERANCES, UNLESS OTHERWISE SPECIFIED		DO NOT SCALE DRAWING FOR DIMENSIONS					
0.XX ± .05		SHEET 1 OF 2			SCALE 1:1		
0.XXX ± .005							
± .1							
INCH [mm]							
CONFIDENTIAL DISCLOSURE							
THIS DRAWING IS THE PROPERTY OF POWEREX INC. OF HARRISON HOLDINGS, INC. AND IS SUBJECT TO RETURN ON DEMAND. ITS CONTENTS ARE CONFIDENTIAL AND MUST NOT BE COPIED OR SUBMITTED TO OUTSIDE PARTIES FOR USE OR EXAMINATION.							
ITEM ID: 761018		AUTHOR Shastri, Balachandra		REVISION DATE 07/25/25		APPROVALS / FILED IN PLM	
MATERIAL: ---		 150 PRODUCTION DRIVE, HARRISON OH 45030 (888) 765-7979					
DESCRIPTION							
7.5HP MED OPEN SCROLL TRIPLEX 240GAL EX4 DUPLEX DESICCANT							
DRAWING NUMBER MST07C6xP5-EX4		REVISION B		SIZE D			

MST07C6xP5-EX4


7.5HP MED OPEN SCROLL TRIPLEX 240GAL EX4 DUPLEX DESICCANT

REVISION NOTES	
DESCRIPTION	ECN
PRODUCTION RELEASE	PXEC0318

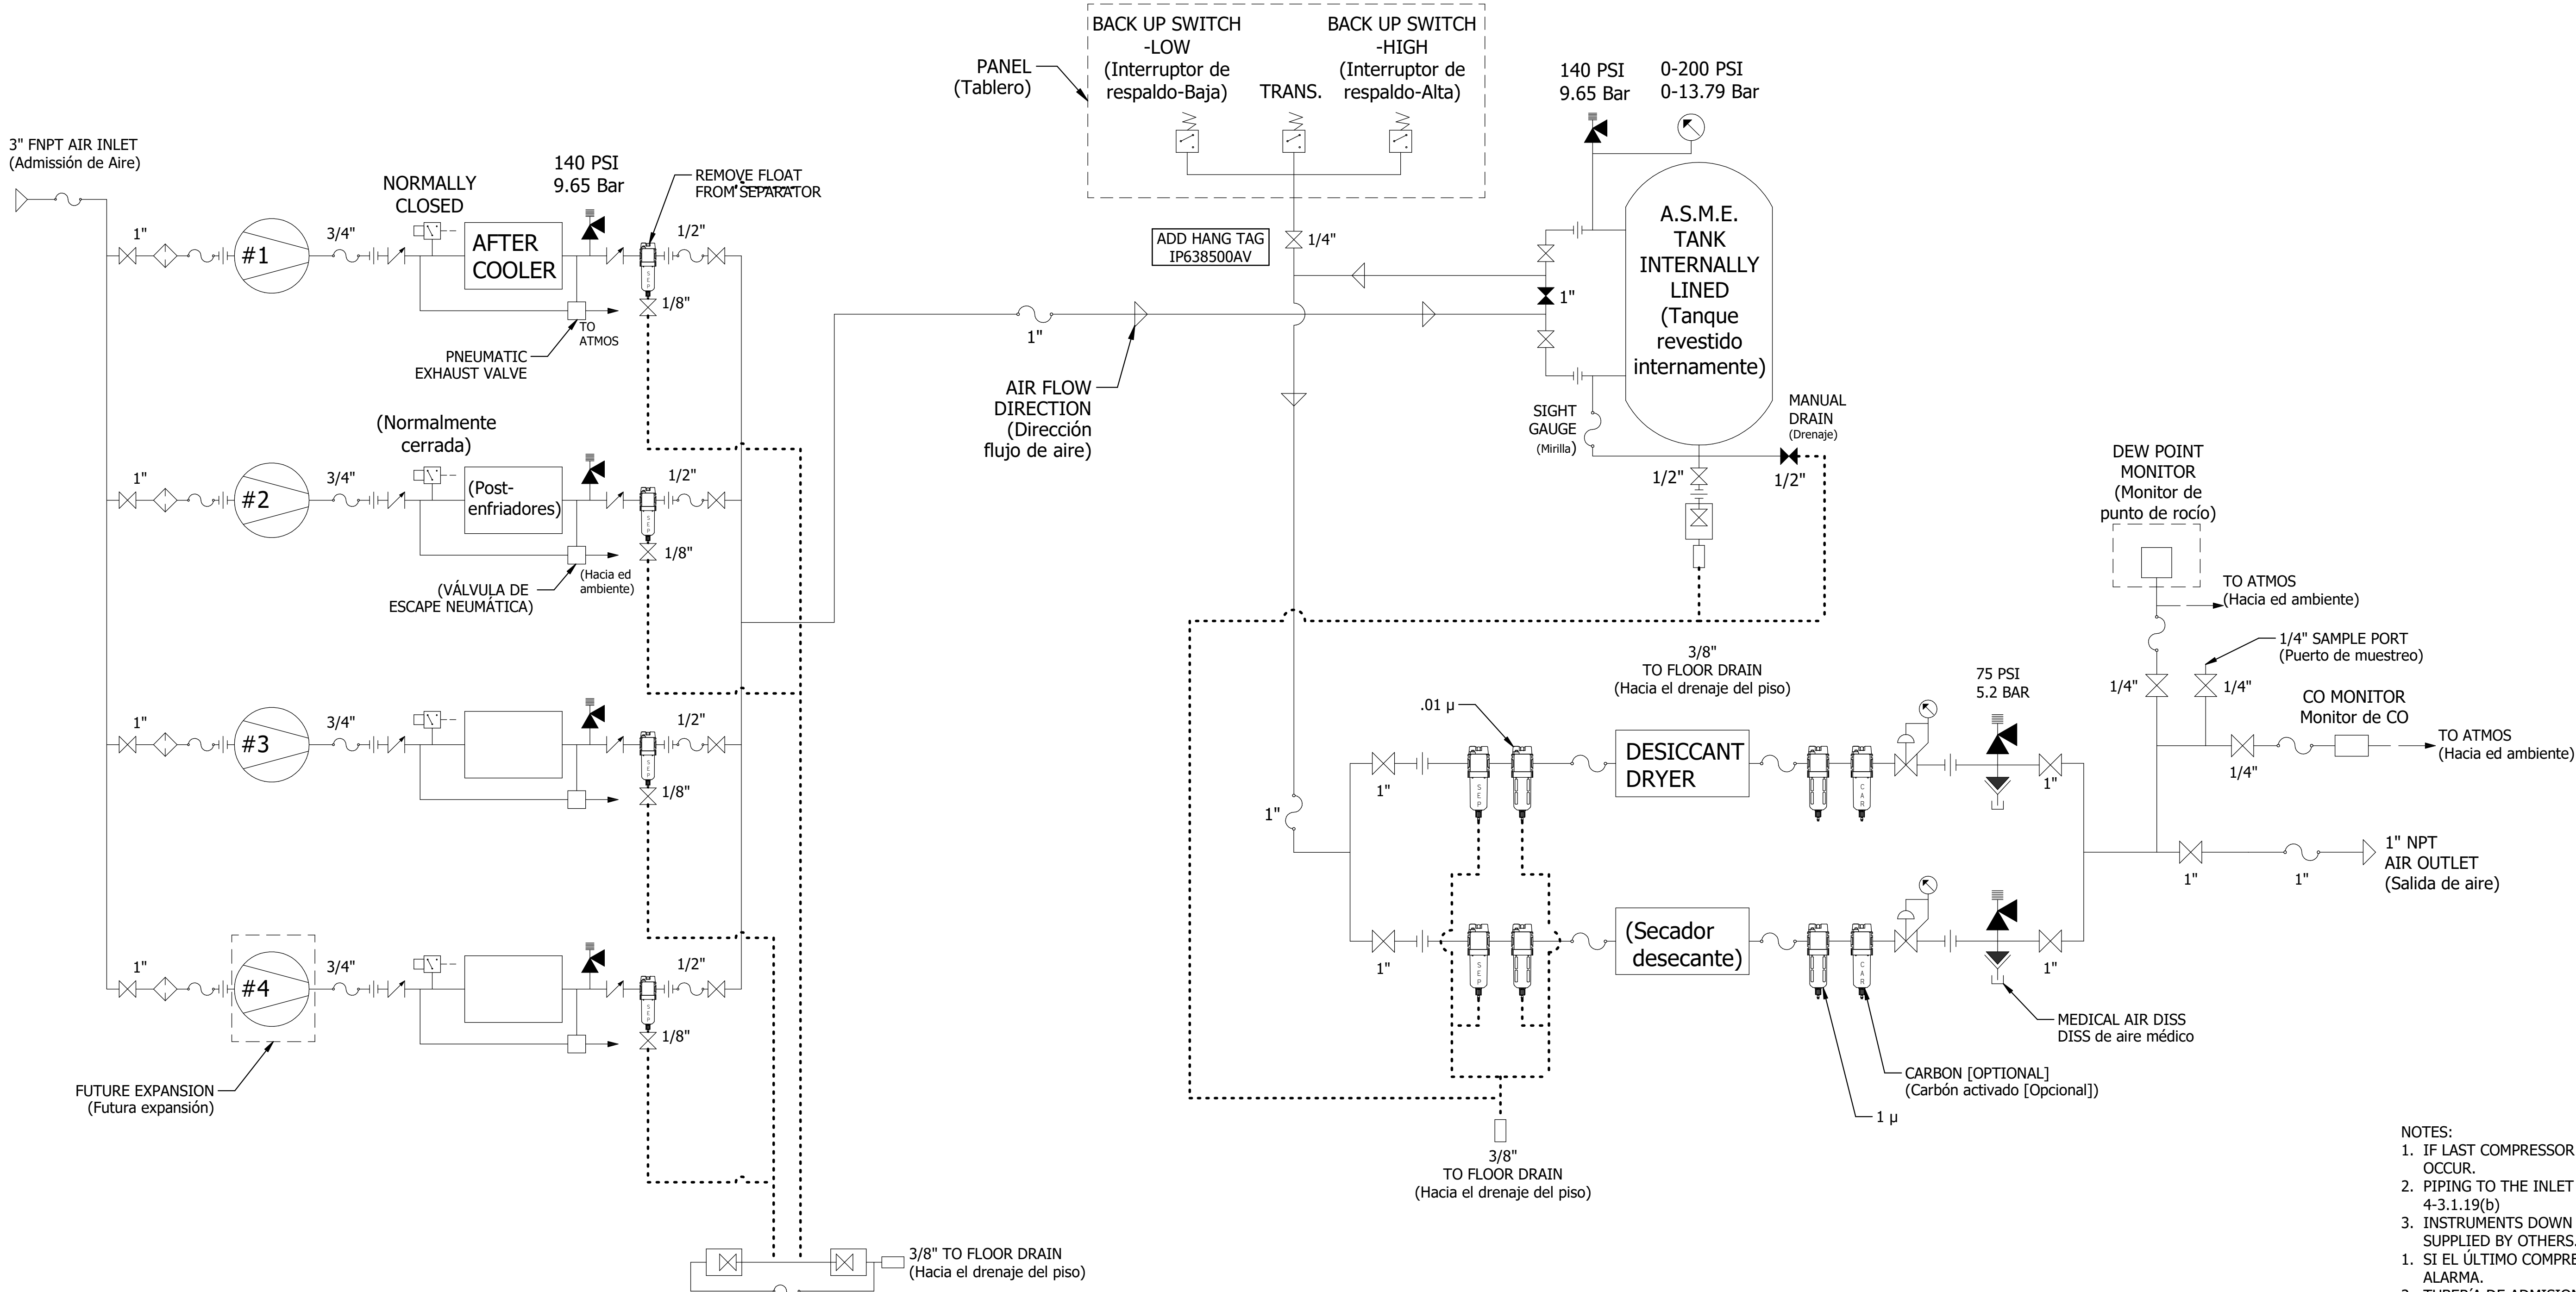

- NOTES:
- IF LAST COMPRESSOR PLEX IS ENERGIZED ALARM WILL OCCUR.
 - PIPING TO THE INLET BY OTHERS AND TO BE PER NFPA99 4-3.1.19(b)
 - INSTRUMENTS DOWN STREAM OF SOURCE VALVE TO BE SUPPLIED BY OTHERS.
 - SI EL ÚLTIMO COMPRESOR SE ACTIVA, SE PRODUCIRÁ UNA ALARMA.
 - TUBERÍA DE ADMISION POR OTROS Y CUMPLIR CON LA NFPA 99 4-3.1.19 (b).
 - ACCESORIOS AGUAS-ABAJO DE LA VALVULA DE CORTE DE SUMINISTRO SERAN INSTALADOS POR OTROS.

LEGEND (Leyenda)			
COMPRESSOR PUMP (Compresor de Aire)	AIR LINE (Tubería de Aire)	BALL VALVE (Válvula bola)	REGULATOR W/ GAUGE (Regulador con Manómetro)
INTAKE FILTER (Filtro admisión)	CONDENSATE LINE (Línea de condensado)	RELIEF VALVE (Válvula de seguridad)	TEMPERTURE SWITCH (Interruptor temperatura)
FILTER/SEPERATOR (Filtro/Seperator)	FLEX HOSE (Manguera flexible)	CHECK VALVE (Válvula Cheque)	PRESSURE SWITCH/TRANSDUCER (Interruptor/Transductor presión)
GAUGE (Manómetro)	UNION (Unión)	DEMAND VALVE (Válvula de demanda)	ELECTRIC AUTO DRAIN (Electroválvula de Drenaje)

SYMBOL LEGEND		DRAWINGS TO CONFORM TO CURRENT REVISION OF THE FOLLOWING AAS STANDARDS: Y14.3 MULTI AND SECTIONAL VIEW DWGS Y14.5 DIMENSIONING AND TOLERANCING	
			
TOLERANCES, UNLESS OTHERWISE SPECIFIED		DO NOT SCALE DRAWING FOR DIMENSIONS	
0.XX ± .05		SHEET 2 OF 2	
0.XXX ± .005			
± .1		SCALE 1:1	
CONFIDENTIAL DISCLOSURE		AUTHOR	
This drawing is the property of POWEREX INC. of HARMON HOLDINGS, INC. and is subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.		REVISION DATE	
		APPROVALS ON FILE IN PLM	
761018		Shastri, Balachandra 07/25/25	
ITEM ID:		POWEREX®	
MATERIAL:		150 PRODUCTION DRIVE, HARRISON OH 45030 (888) 766-7979	
DESCRIPTION		DRAWING NUMBER	
7.5HP MED OPEN SCROLL TRIPLEX 240GAL EX4 DUPLEX DESICCANT		MST07C6xP5-EX4	
		REVISION	
		B	
		D	

