



REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK



FIELD FURNISHED
DISCONNECT IS
REQUIRED

SEE NOTES ON
DATA TABLE PAGE

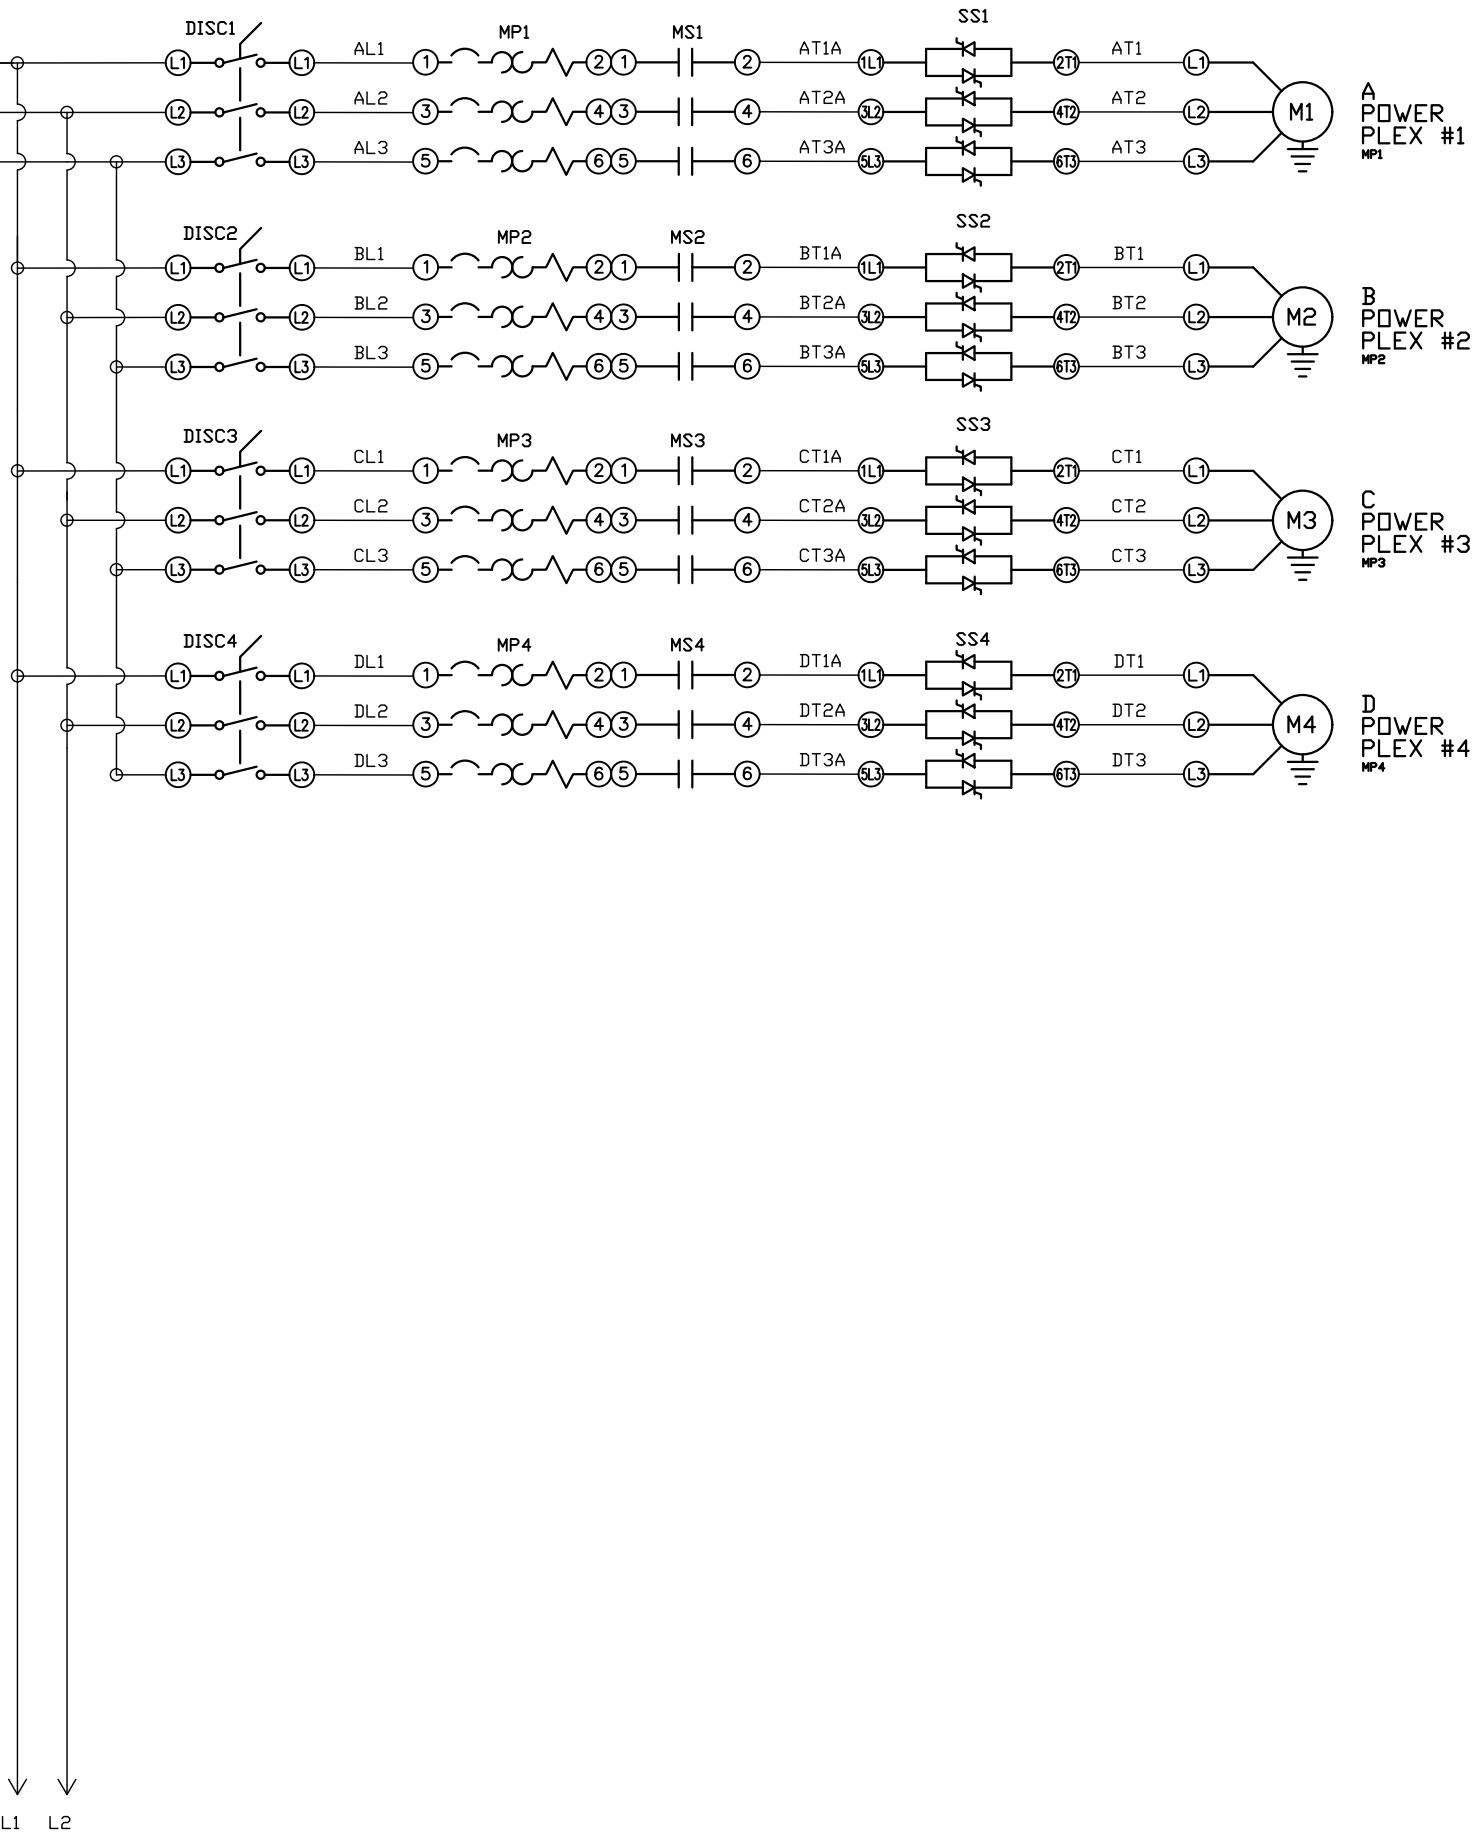

OPTIONAL:

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25

PANEL TYPE

QUADPLEX LAB COMP

HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO


DWG. TYPE WIRING

DWG. NO.

PXMI-LAS416

SHEET	SIZE
W-1	B

PXMI-LAS416

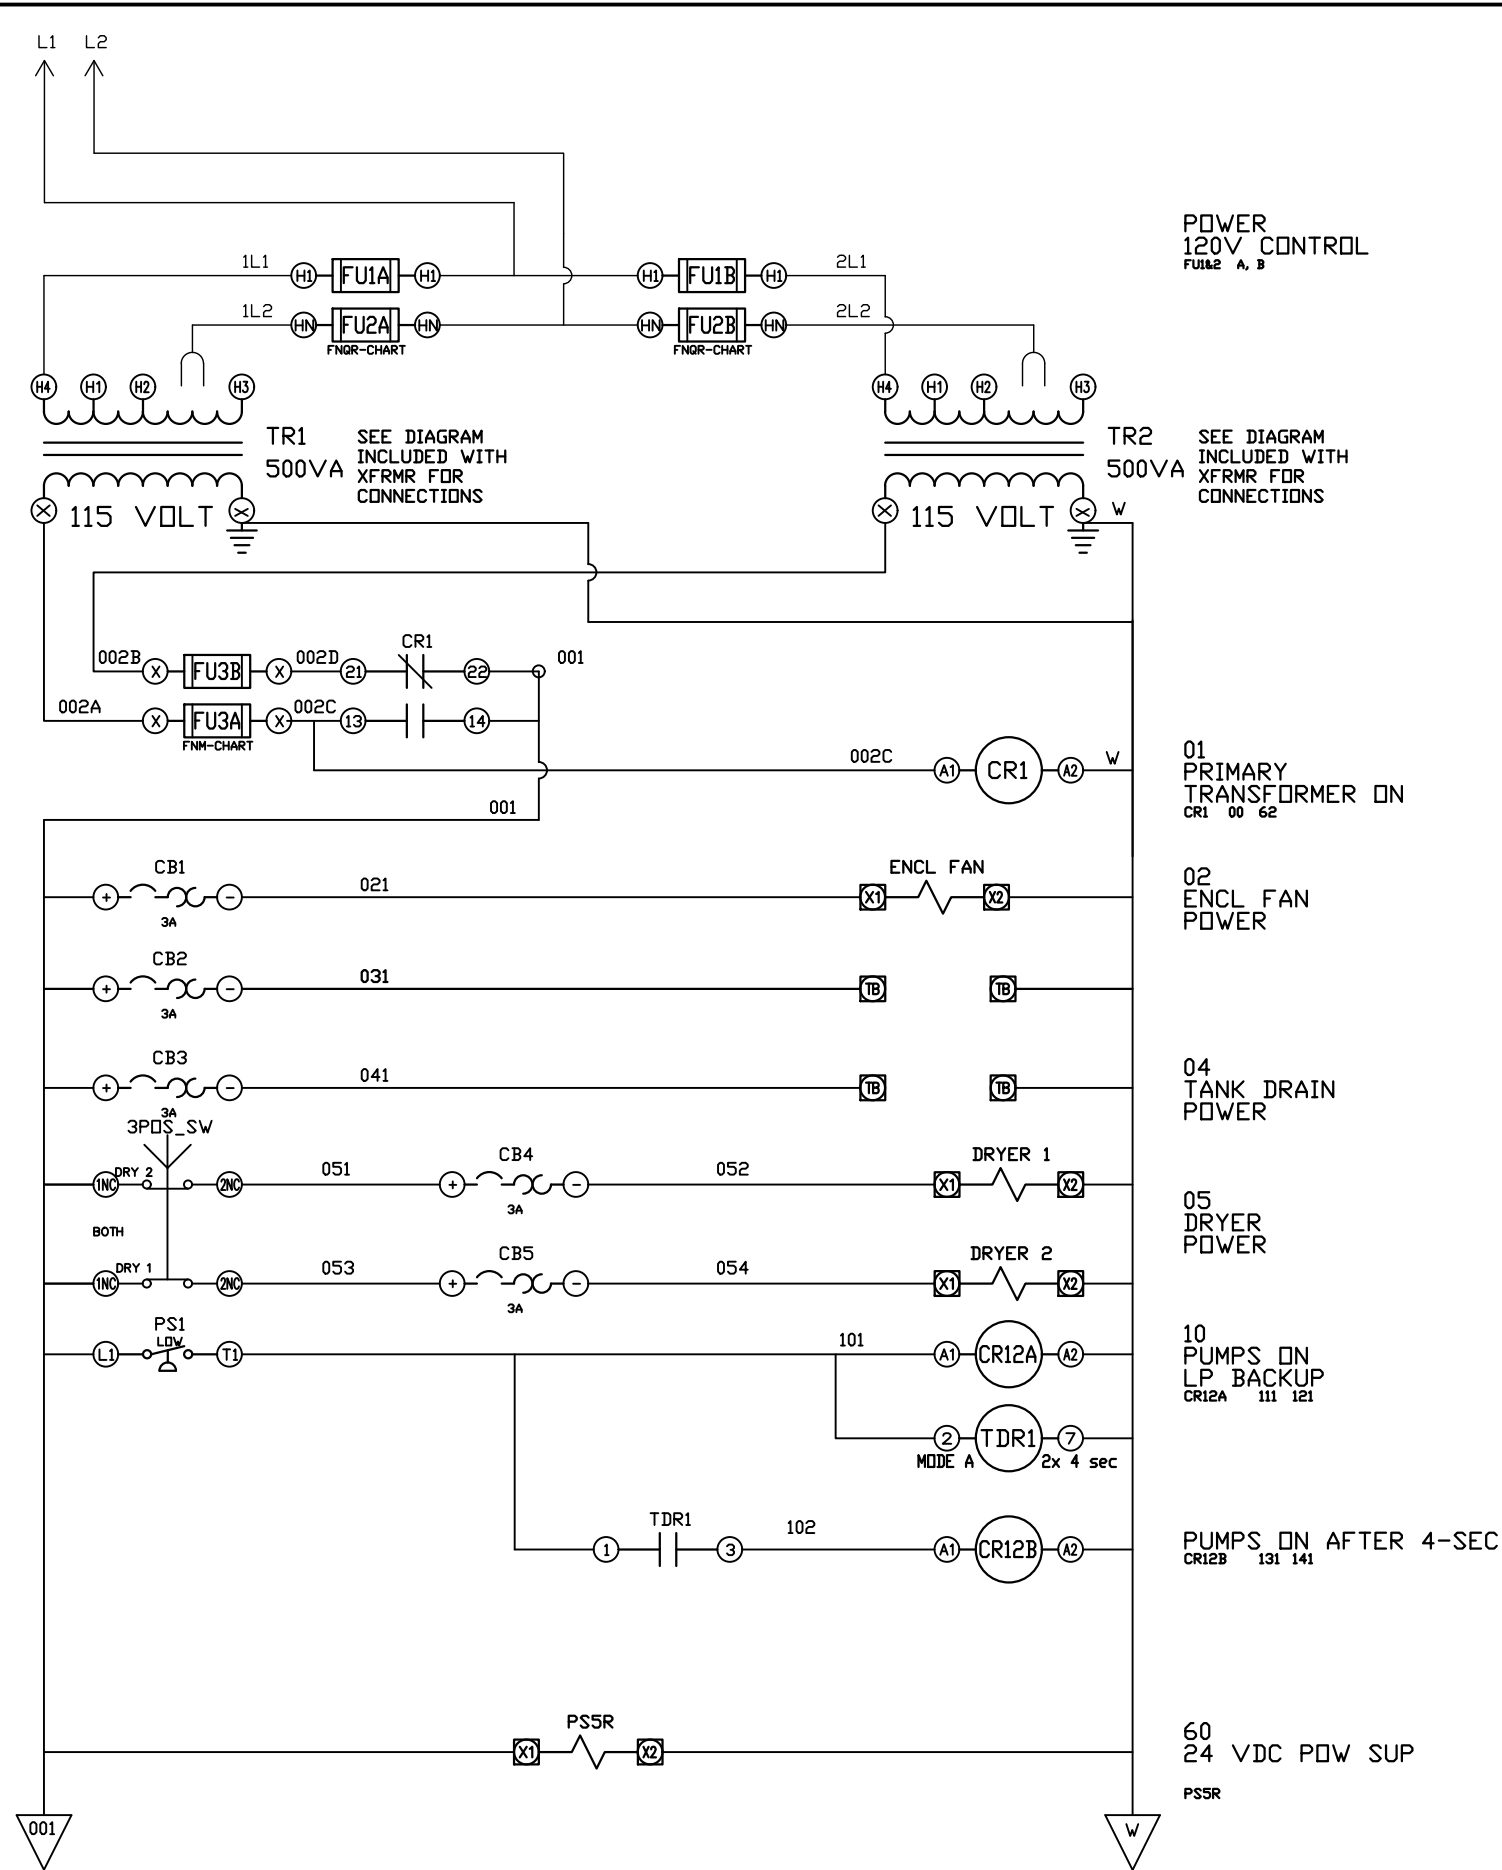

POWER
120V CONTROL
FU1&2 A, B

SEE DIAGRAM
INCLUDED WITH
XFRMR FOR
CONNECTIONS

01
PRIMARY
TRANSFORMER ON
CR1 00 62

02
ENCL FAN
POWER

04
TANK DRAIN
POWER

05
DRYER
POWER

10
PUMPS ON
LP BACKUP
CR12A 111 121

PUMPS ON AFTER 4-SEC
CR12B 131 141

60
24 VDC POW SUP
PS5R

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

OPTIONAL:

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25

PANEL TYPE

QUADPLEX LAB COMP

HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO

DWG. TYPE WIRING



DWG. NO.

PXMI-LAS416

SHEET	SIZE
W-2	B

PXMI-LAS416

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

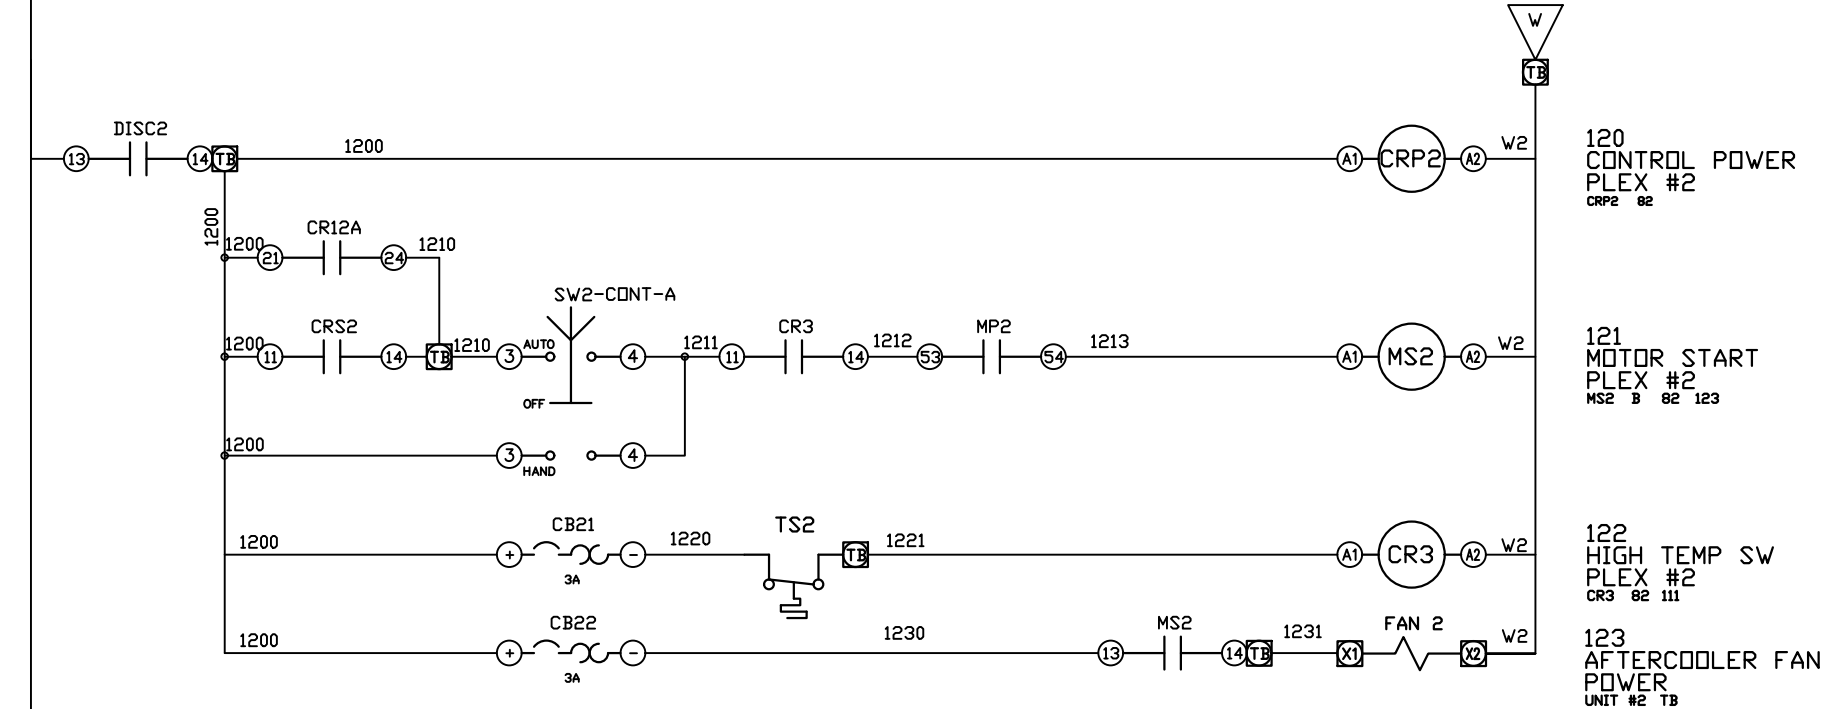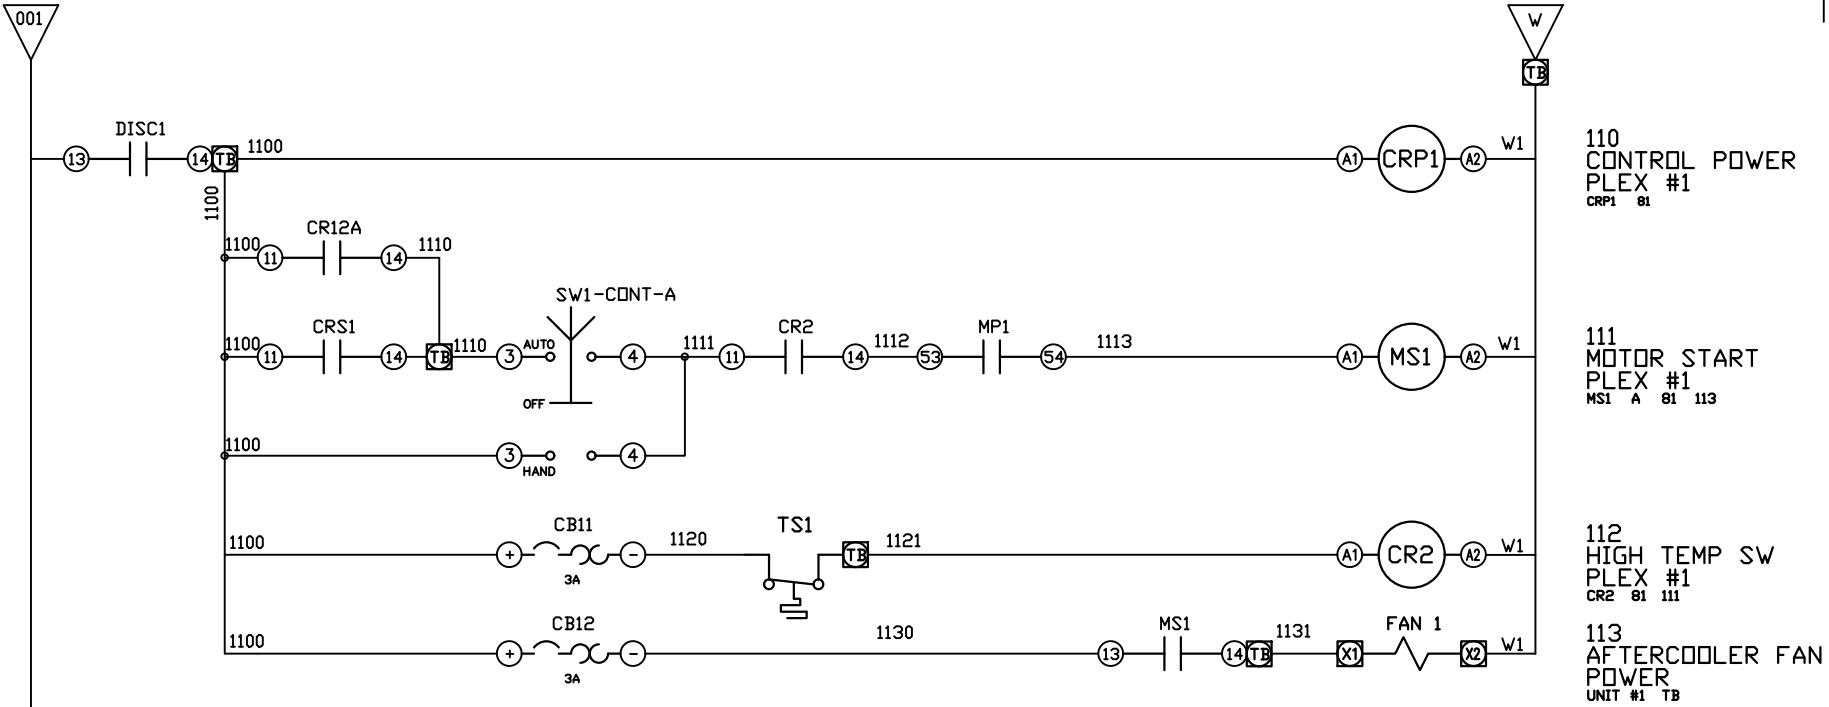

OPTIONAL:

POWEREX™

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25



PANEL TYPE
QUADPLEX LAB COMP
HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO

DWG. TYPE
WIRING

DWG. NO.
PXMI-LAS416

SHEET	SIZE
W-3	B

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

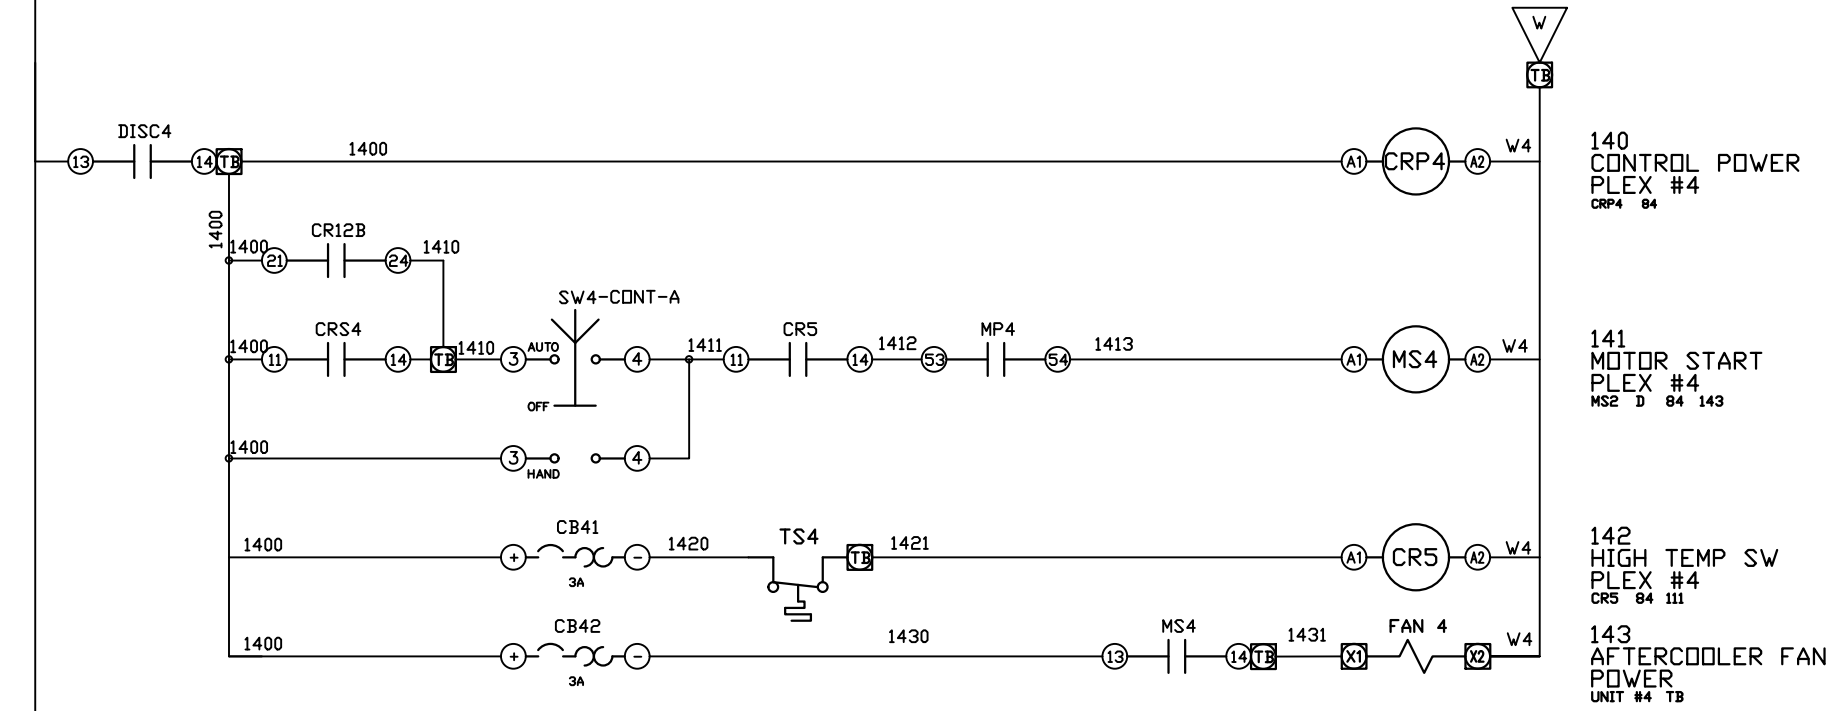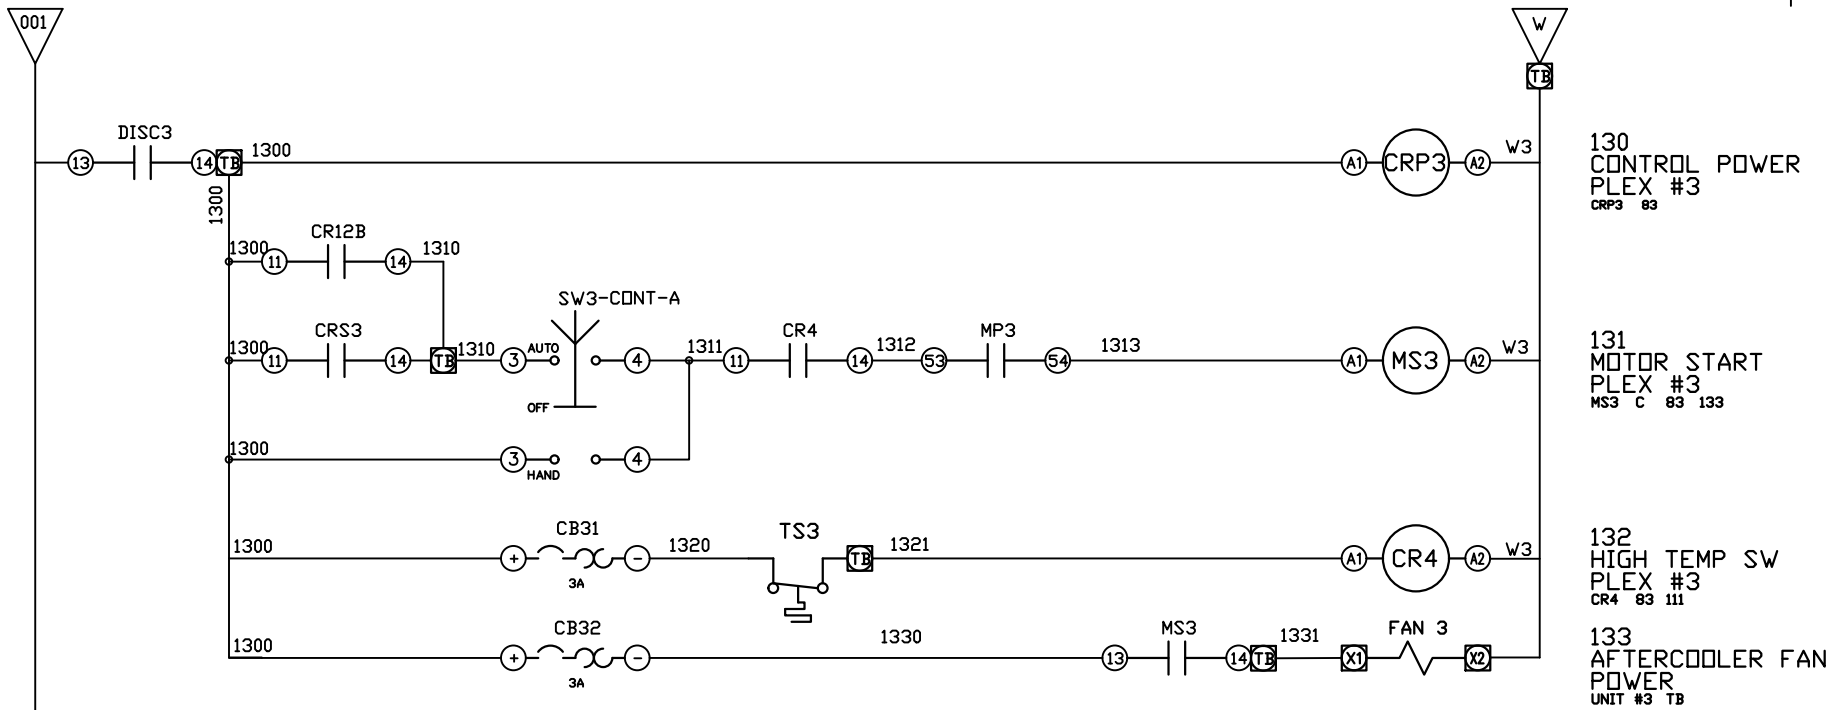

OPTIONAL:

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25

PANEL TYPE
QUADPLEX LAB COMP
HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO



DWG. TYPE
WIRING

DWG. NO.
PXMI-LAS416

SHEET W-4	SIZE B
--------------	-----------

PXMI-LAS416

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

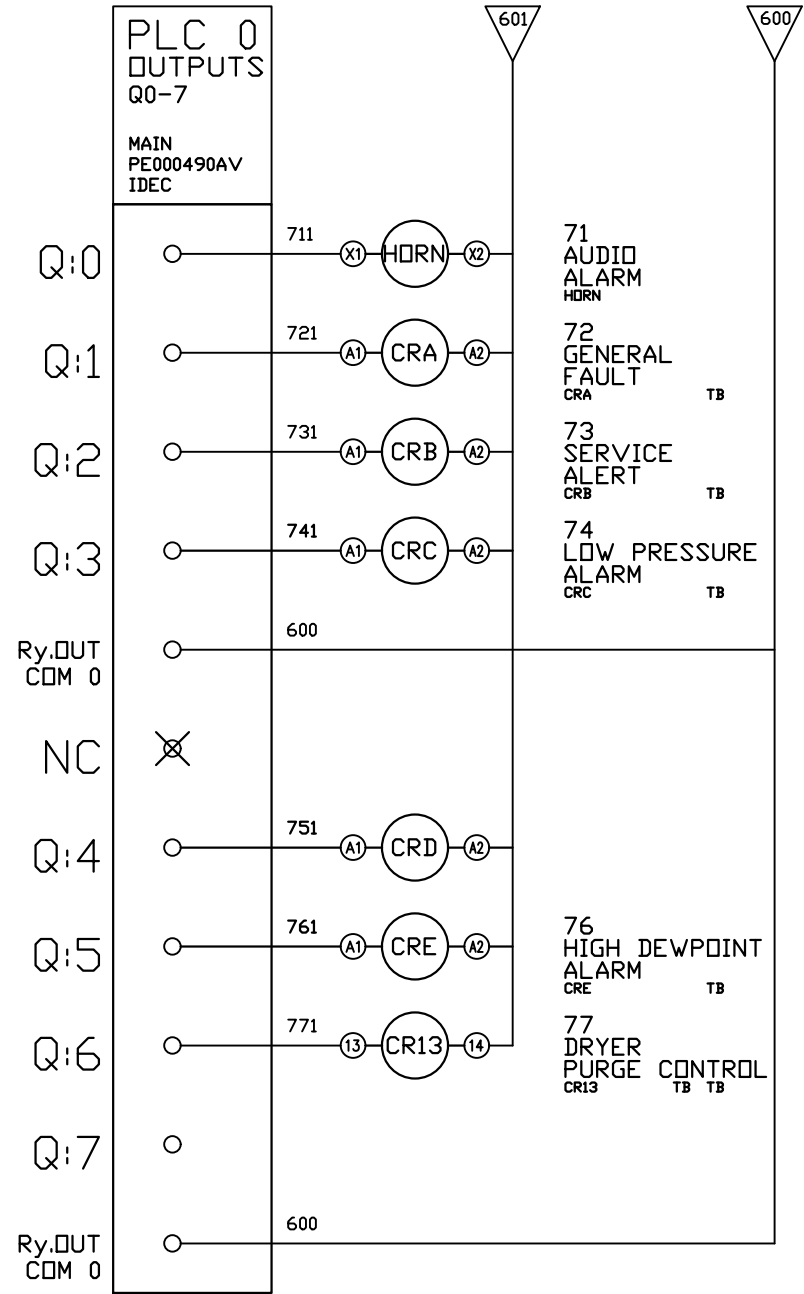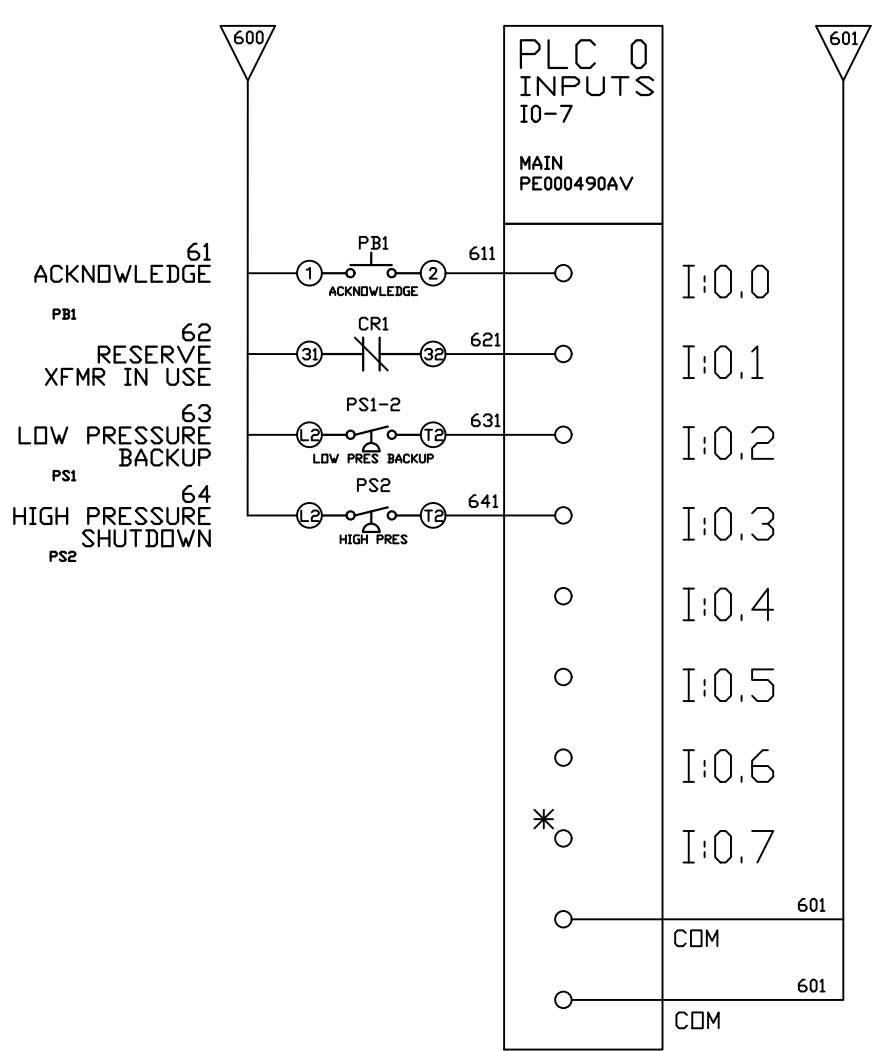

OPTIONAL:

POWEREX™

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25

PANEL TYPE

QUADPLEX LAB COMP

HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO

DWG. TYPE WIRING

DWG. NO.

PXMI-LAS416


SHEET

W-6

SIZE

B

* INSTALL JUMPER FOR FACTORY TEST

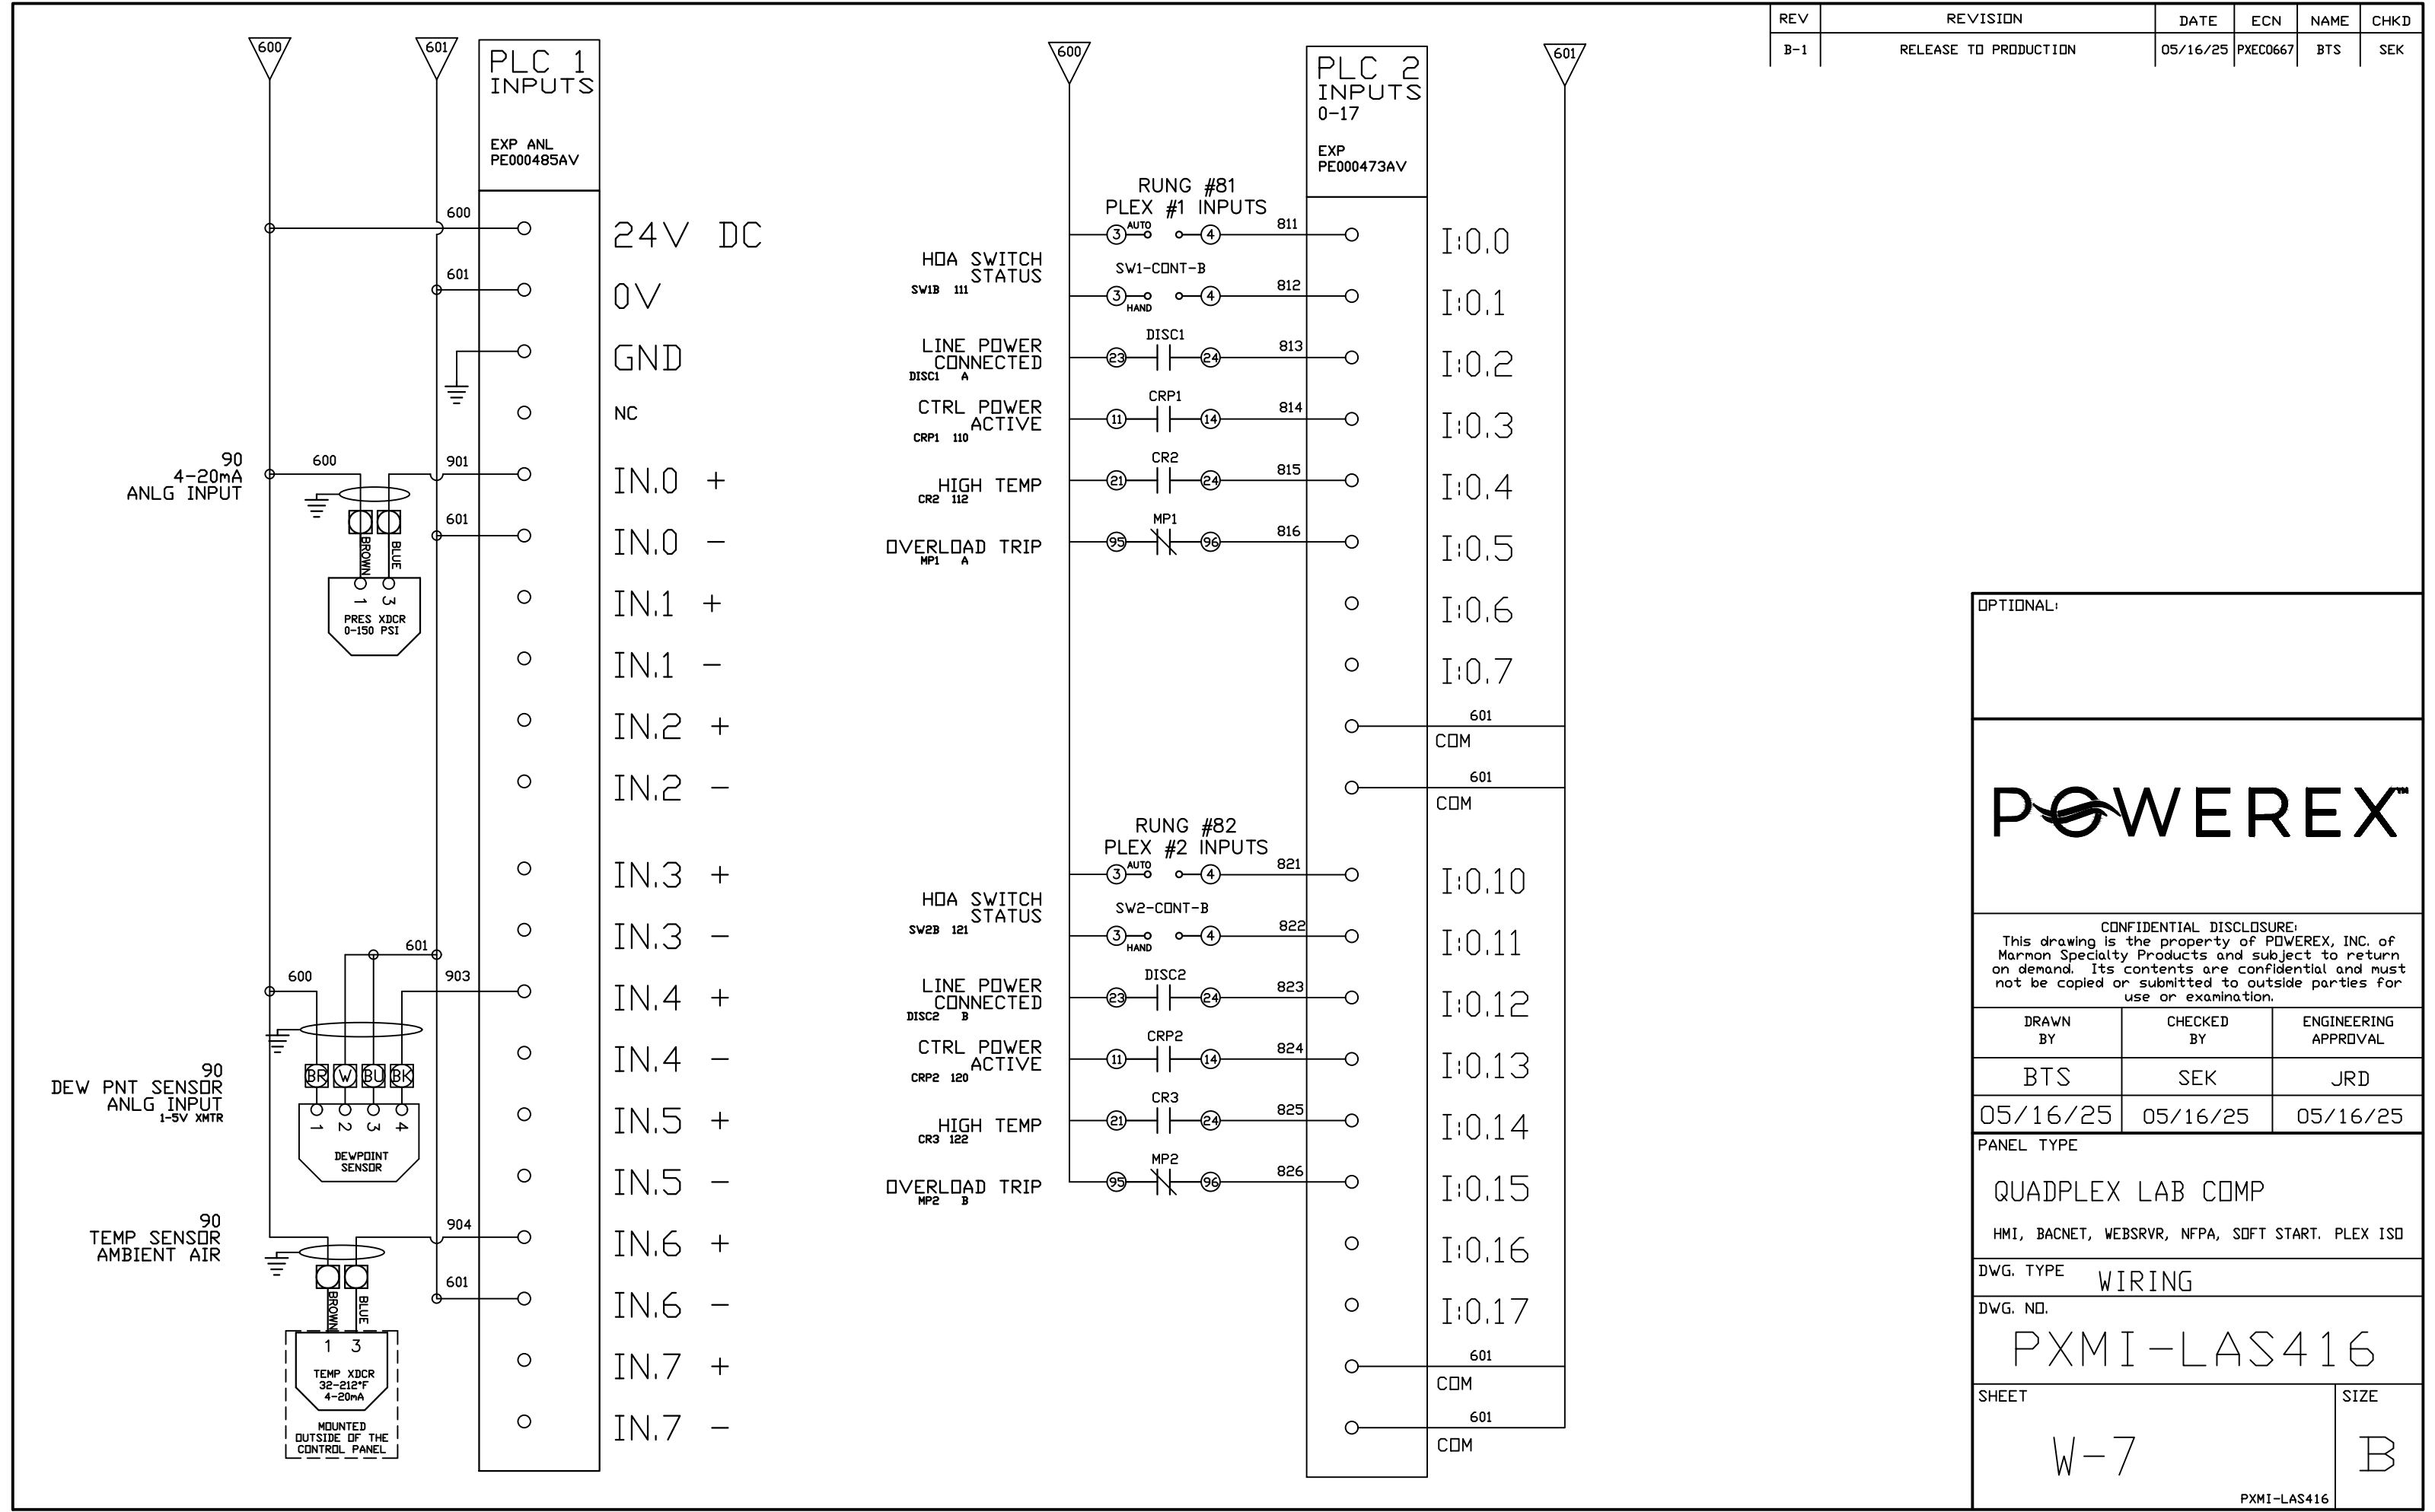

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

OPTIONAL:



CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25

PANEL TYPE

QUADPLEX LAB COMP

HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO

DWG. TYPE

WIRING



DWG. NO.

PXMI-LAS416

SHEET	SIZE
W-7	B

PXMI-LAS416

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

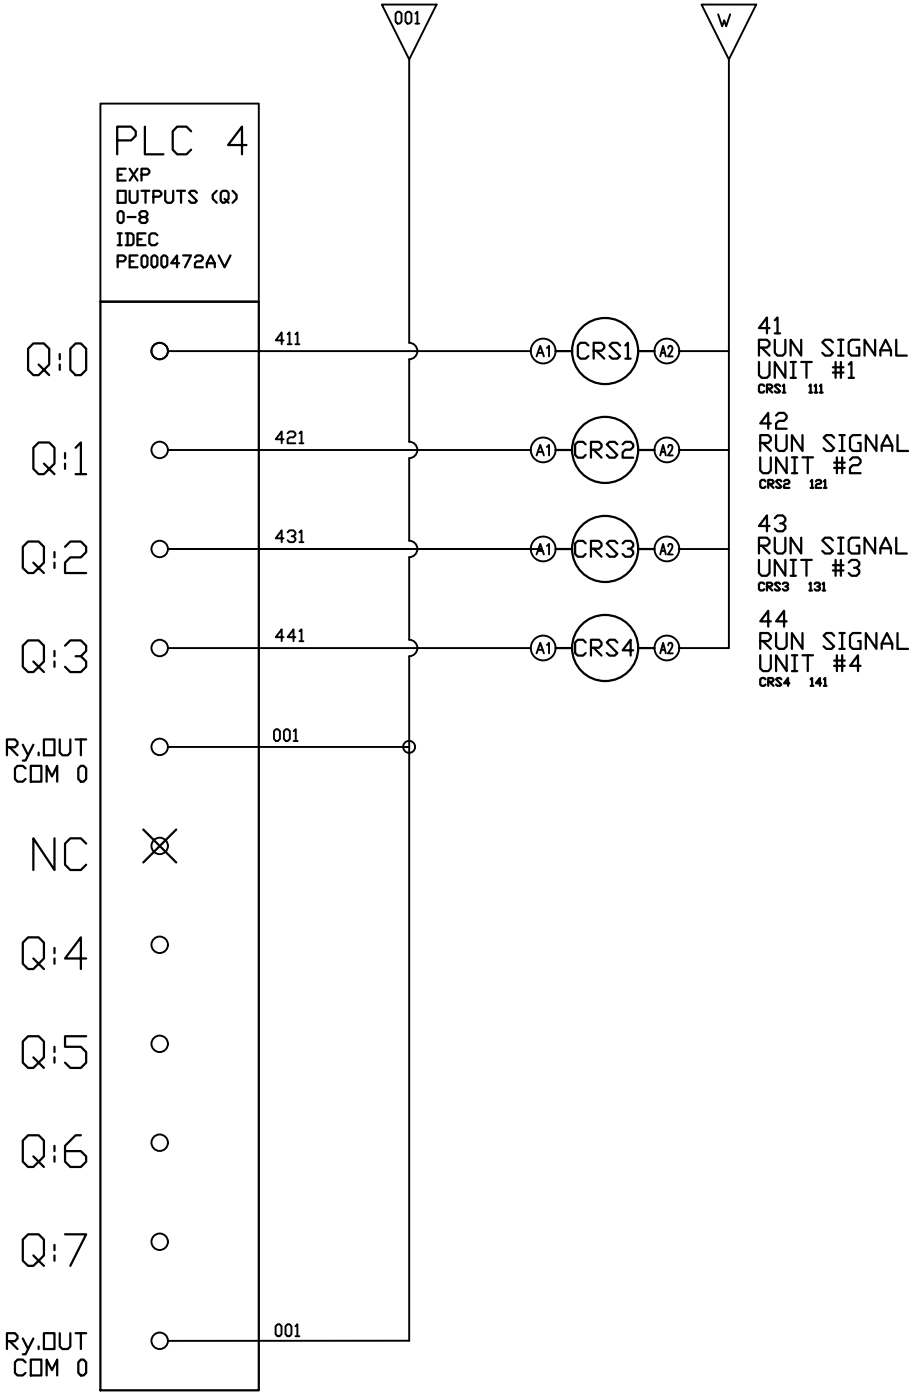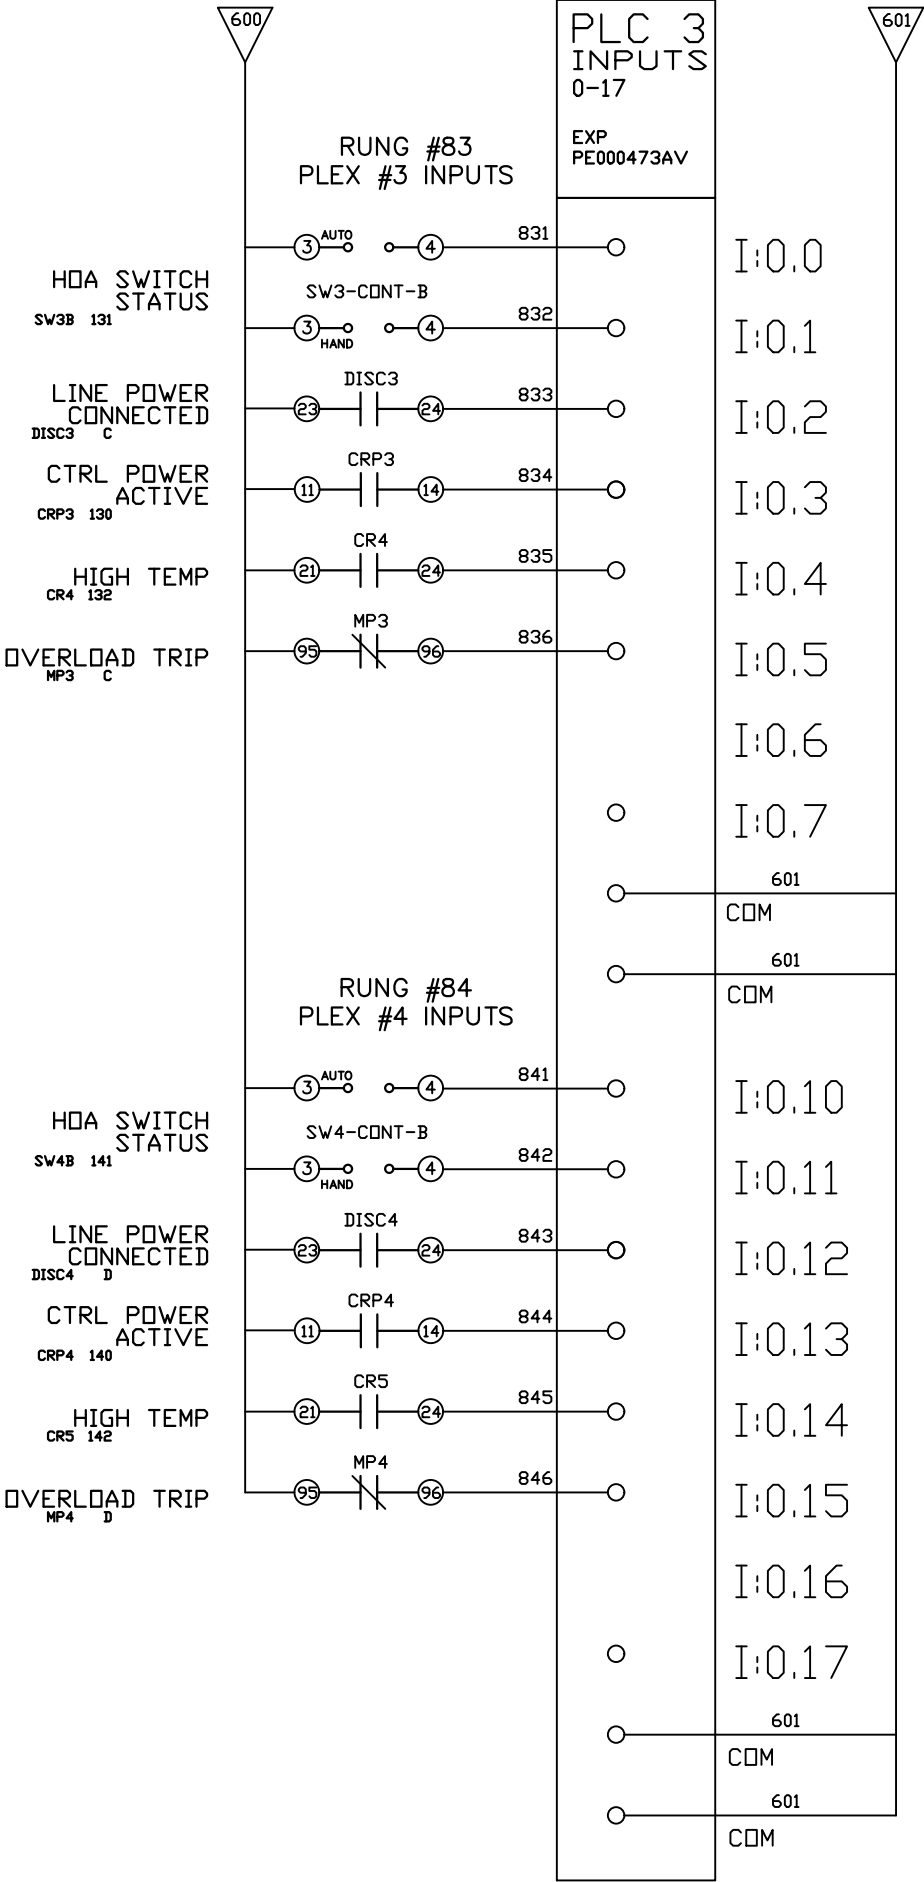

OPTIONAL:

POWEREX™

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of
Marmon Specialty Products and subject to return
on demand. Its contents are confidential and must
not be copied or submitted to outside parties for
use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25

PANEL TYPE

QUADPLEX LAB COMP

HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO

DWG. TYPE WIRING

DWG. NO.

PXMI-LAS416

SHEET

W-8

SIZE


B


SET START TIME TO 3-SEC (B)

SET INITIAL VOLT SETTING TO 67% (D)

SET STOP TIME TO 60 SEC (C)

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

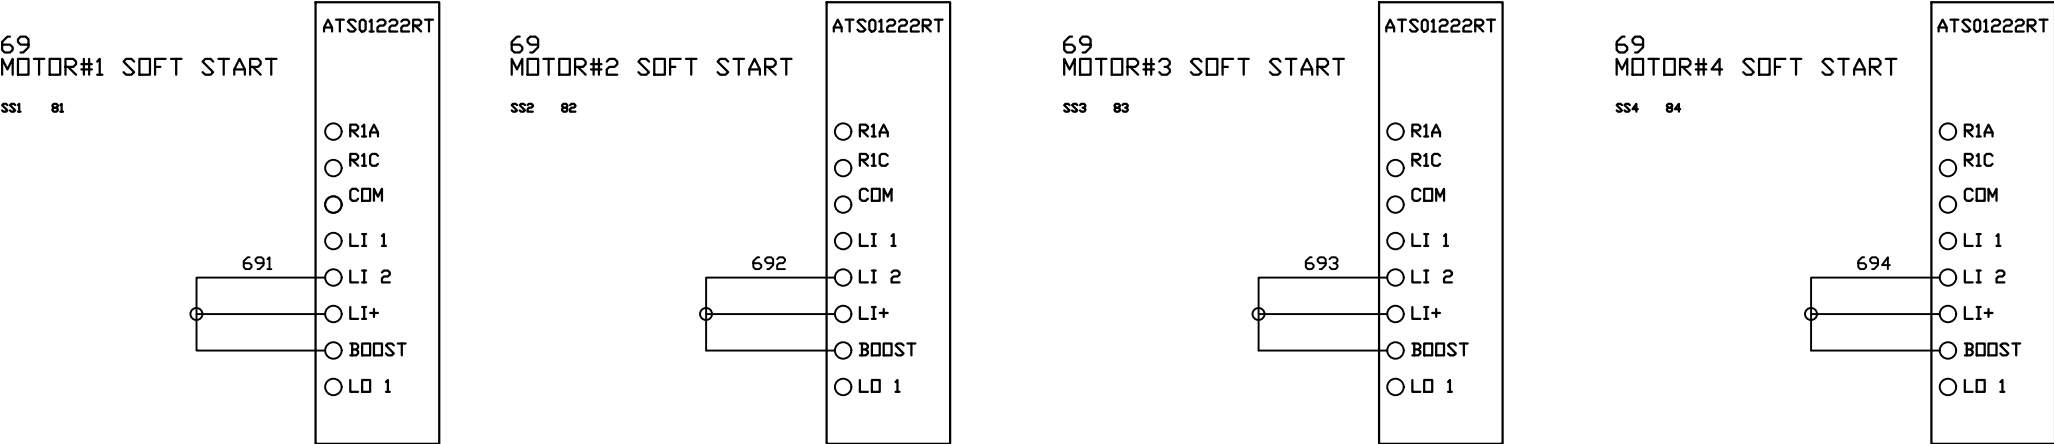

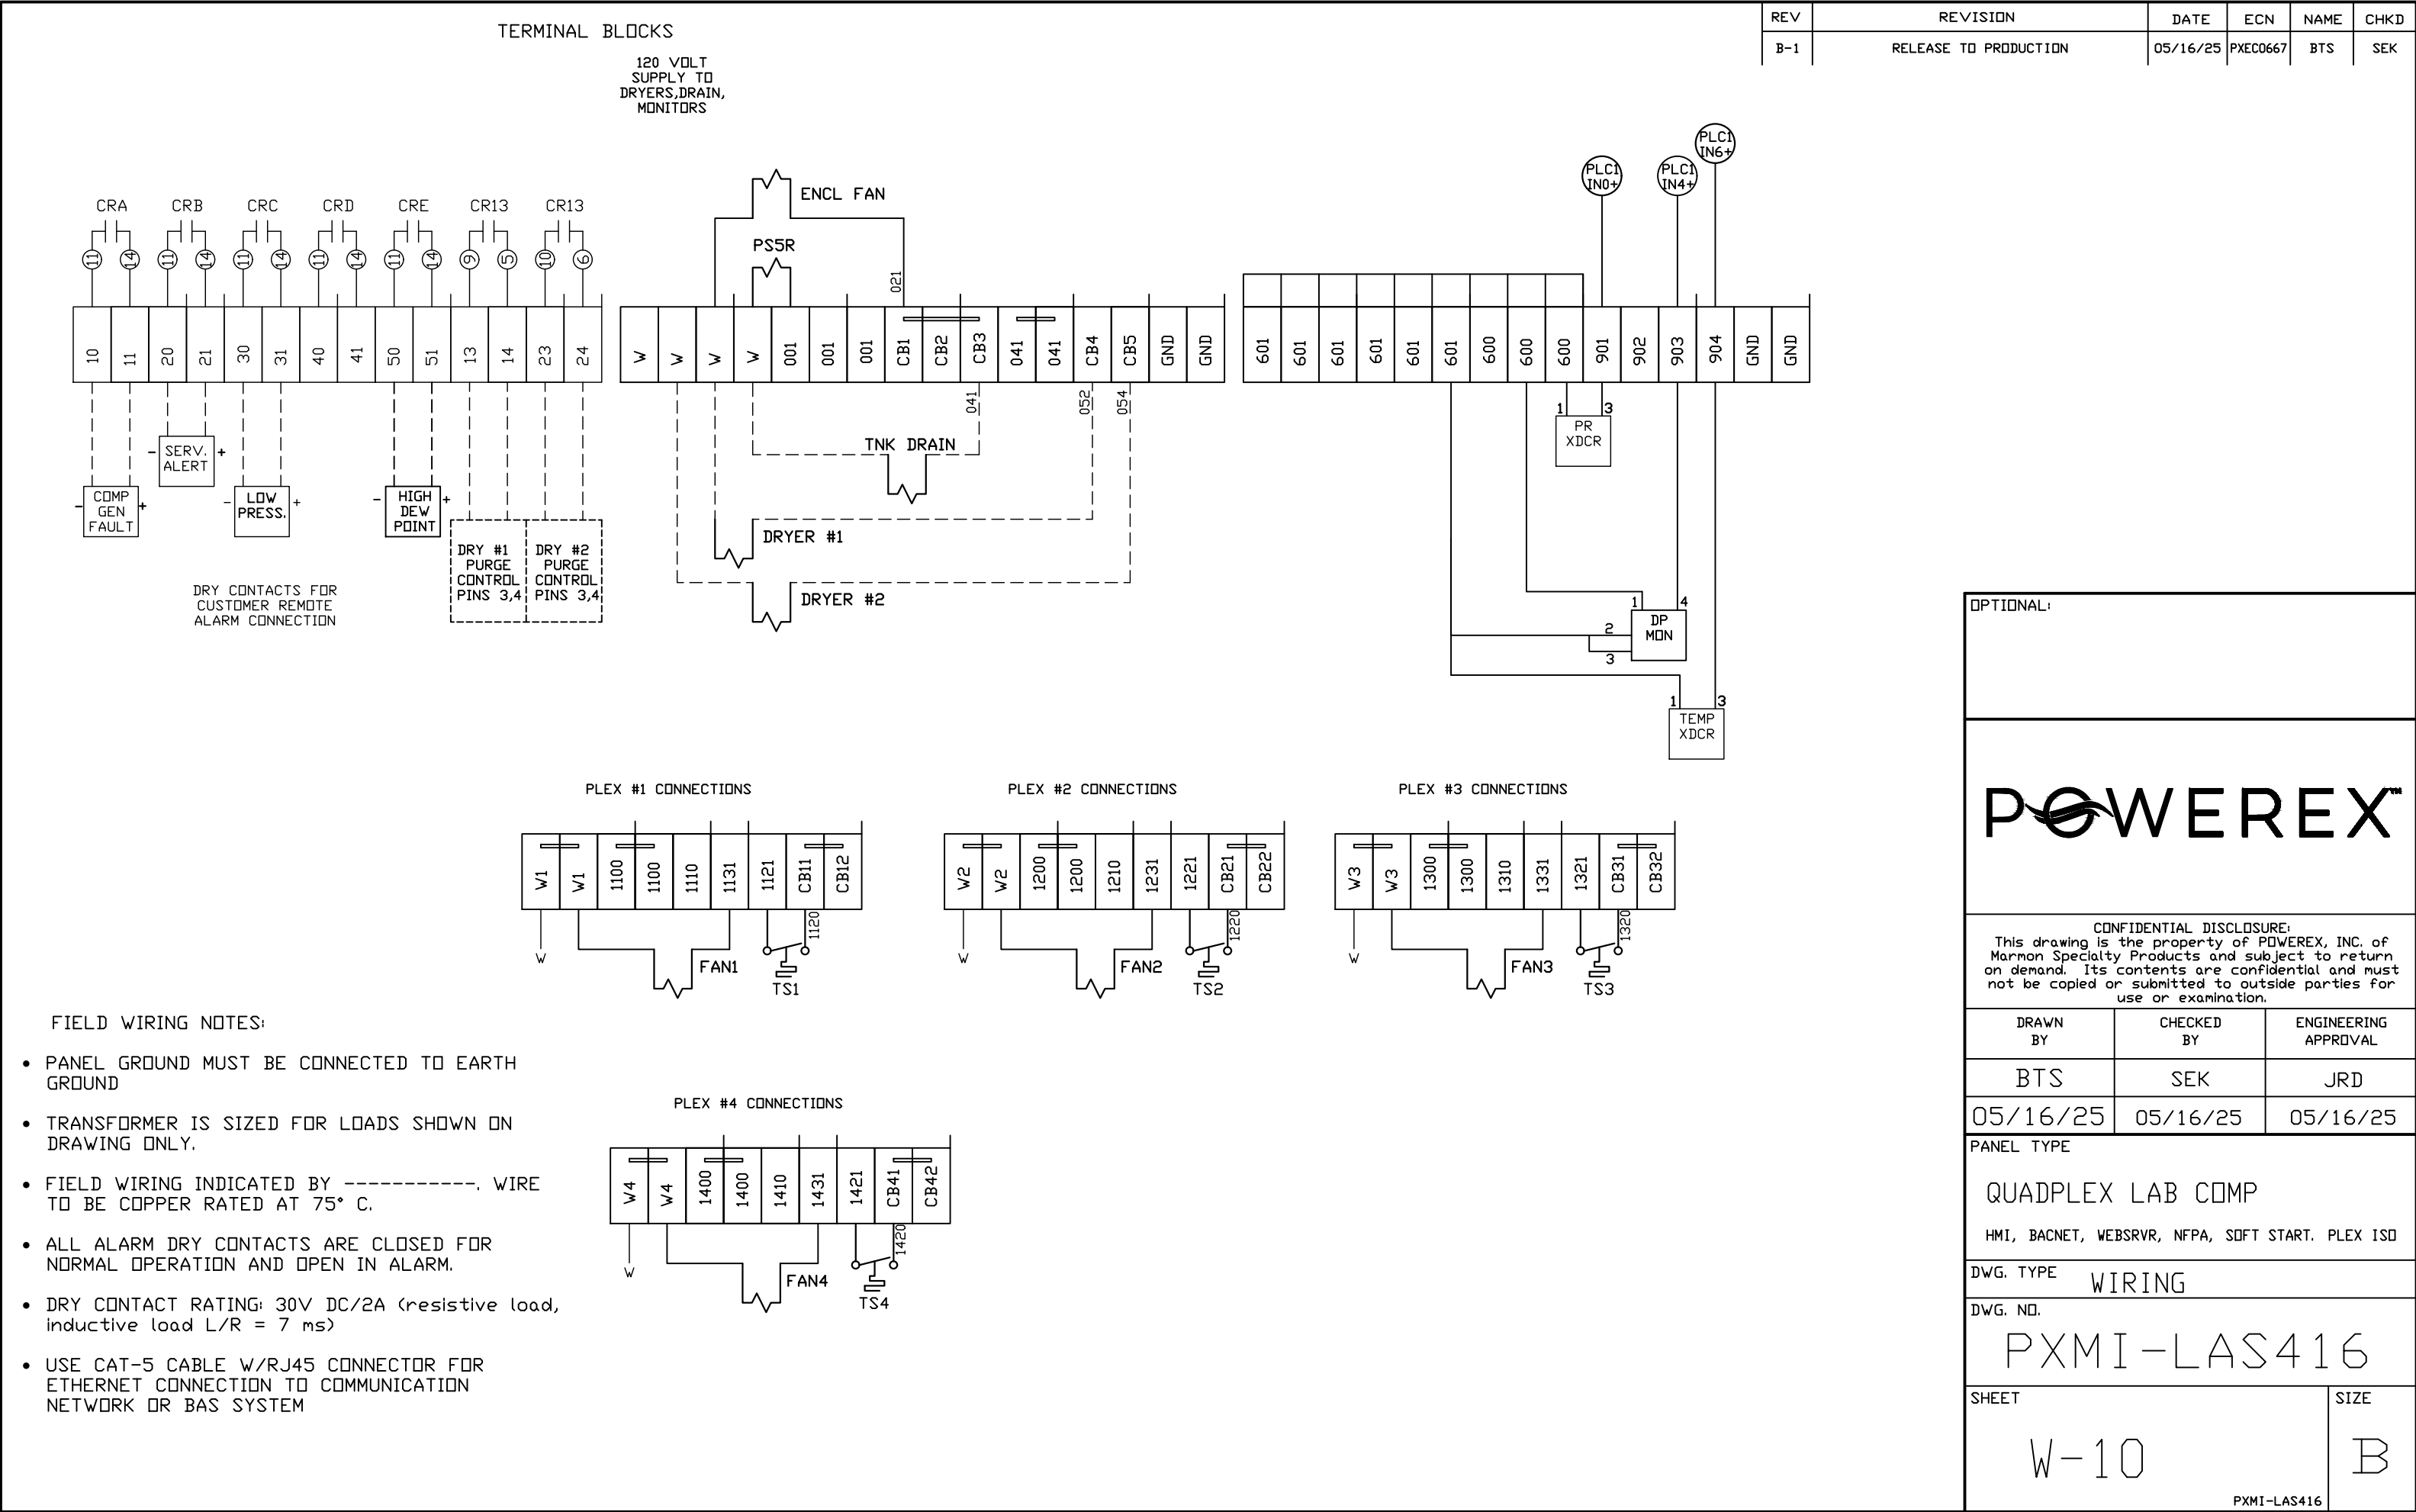

FIELD WIRING NOTES:

PANEL GROUND MUST BE CONNECTED TO EARTH GROUND

TRANSFORMER IS SIZED FOR LOADS SHOWN ON DRAWING ONLY.

FIELD WIRING INDICATED BY -----, WIRE TO BE COPPER RATED AT 75° C.

ALL ALARM DRY CONTACTS ARE CLOSED FOR NORMAL OPERATION AND OPEN IN ALARM.

DRY CONTACT RATING: 30V DC/2A (resistive load, inductive load L/R = 7 ms)

USE CAT-5 CABLE W/RJ45 CONNECTOR FOR ETHERNET CONNECTION TO COMMUNICATION NETWORK OR BAS SYSTEM

OPTIONAL:

POWEREX™

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY

CHECKED BY

ENGINEERING APPROVAL

BTS

SEK

JRD

05/16/25

05/16/25

05/16/25

PANEL TYPE

QUADPLEX LAB COMP

HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO

DWG. TYPE

WIRING

DWG. NO.

PXMI-LAS416

SHEET


W-10

SIZE

B

PXMI-LAS416

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

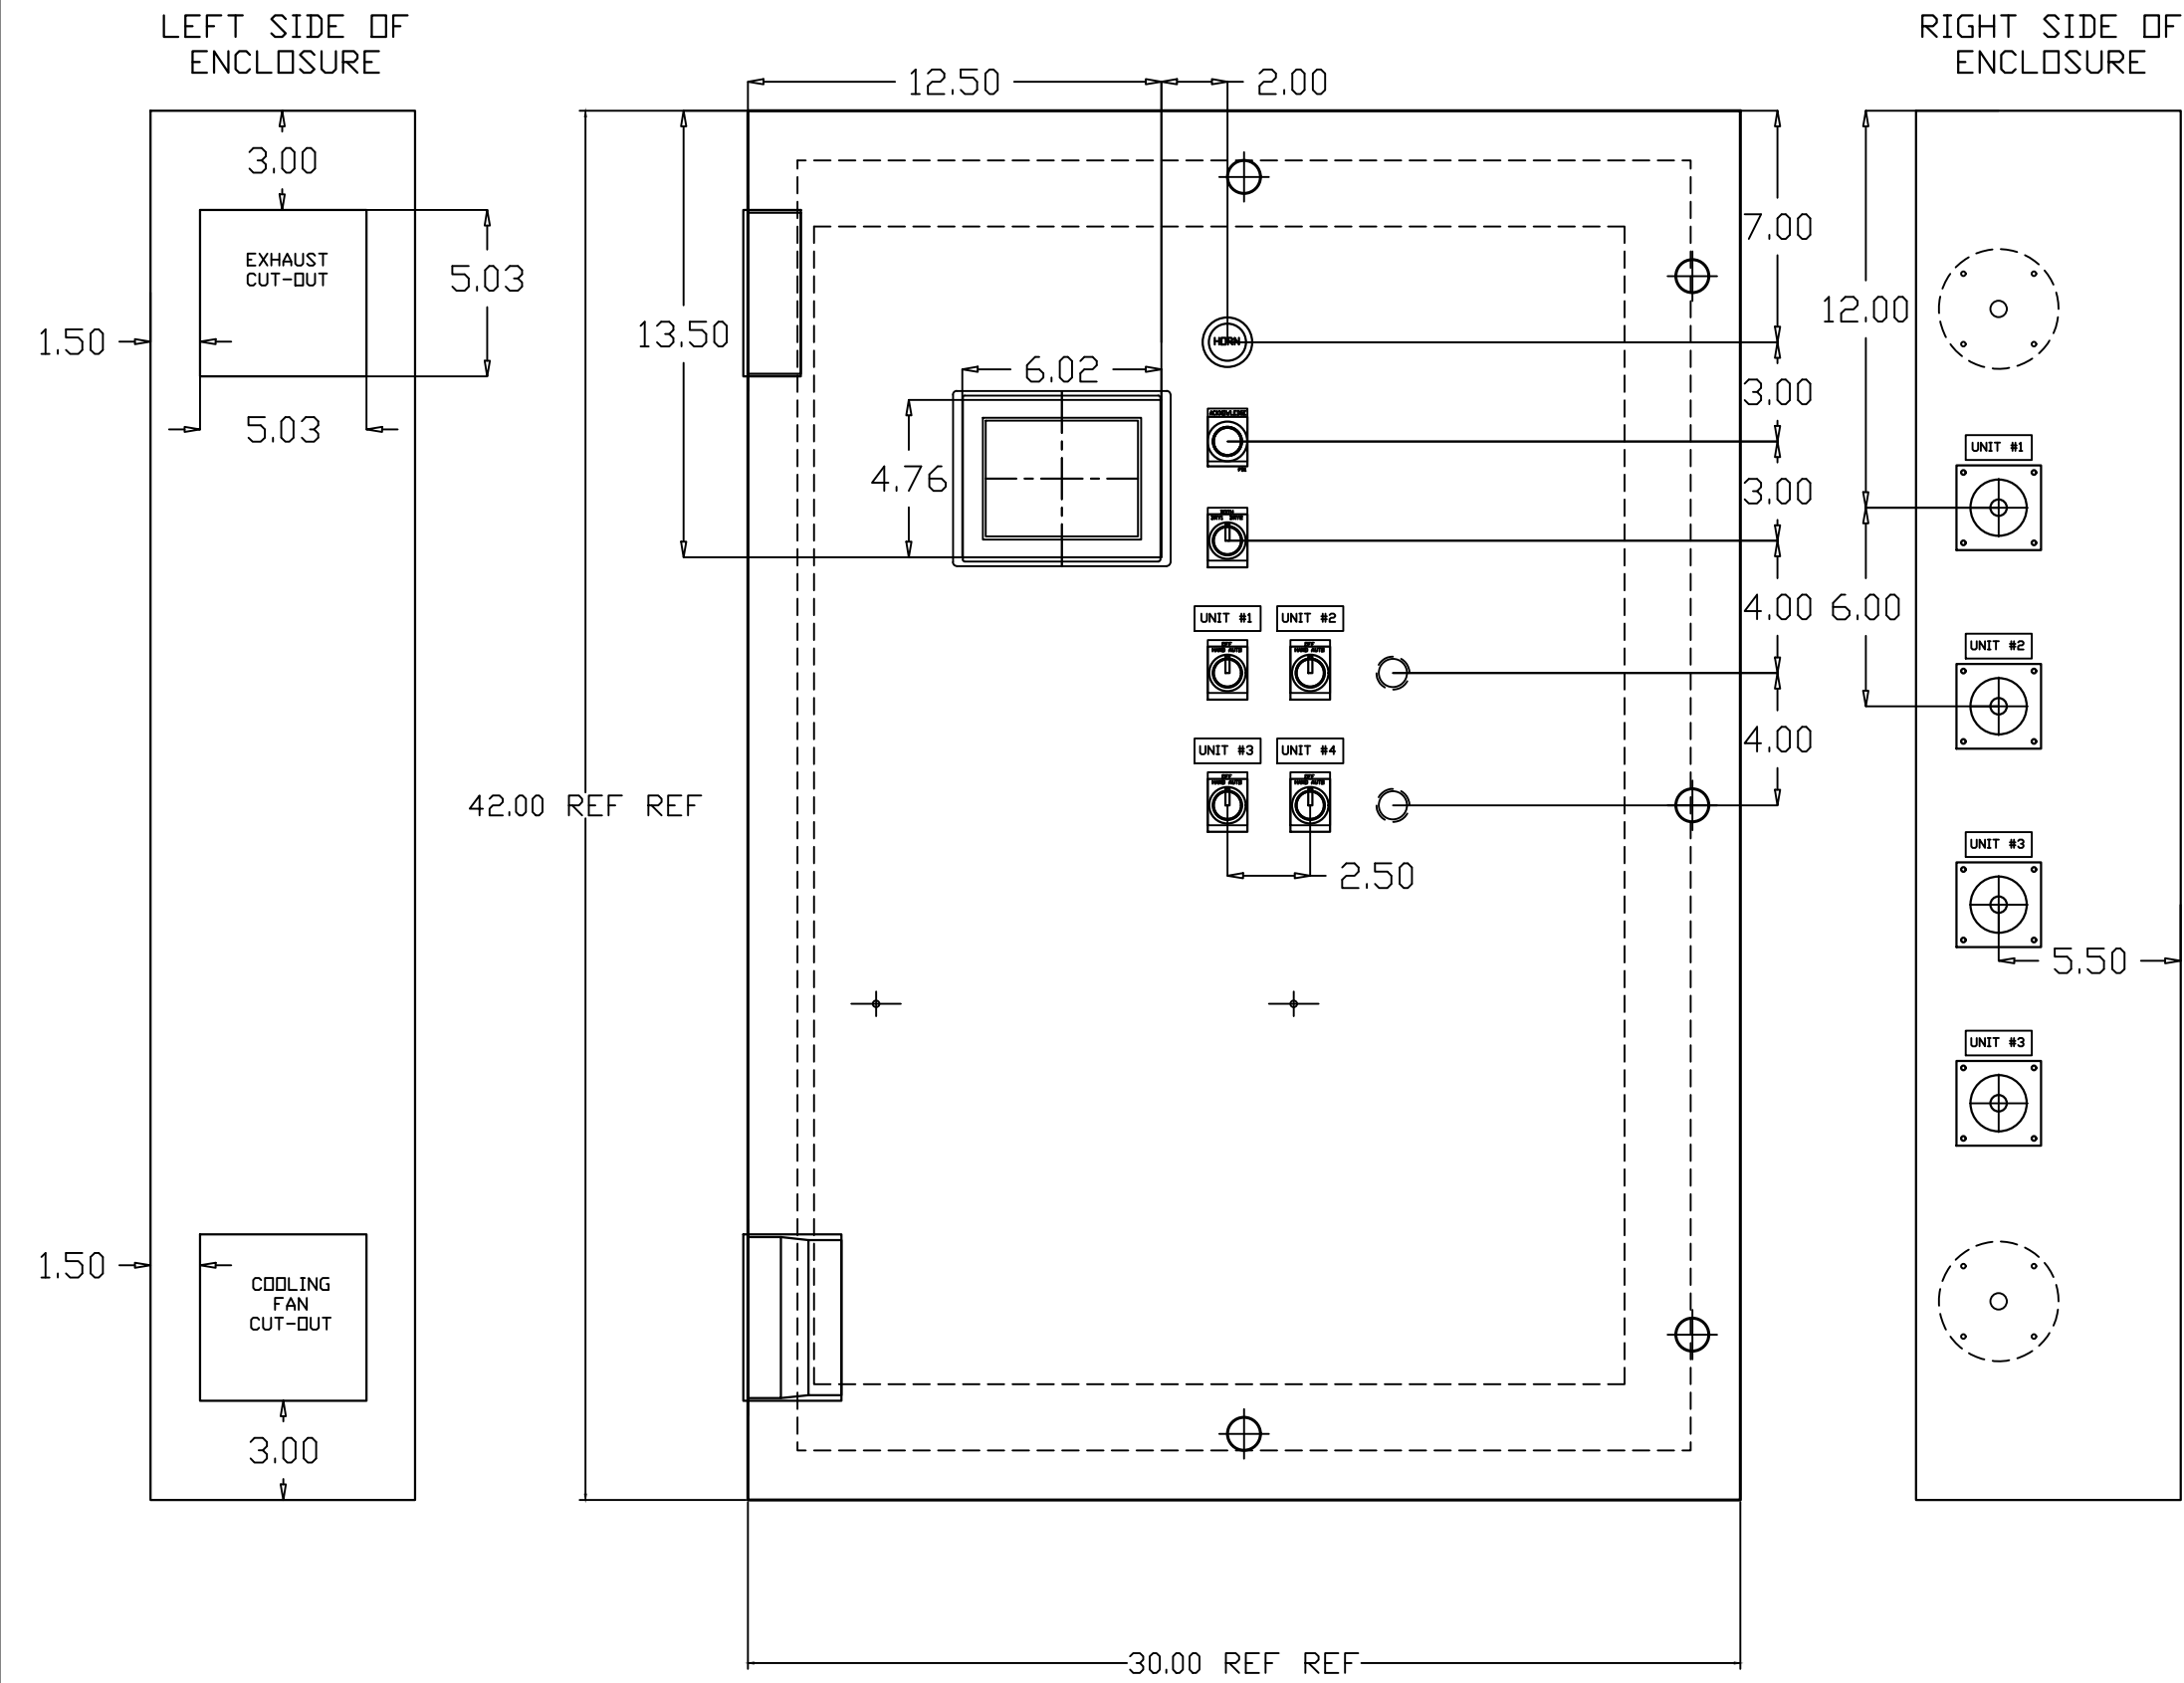

OPTIONAL:

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25

PANEL TYPE

QUADPLEX LAB COMP

HMI, BACNET, WEBSVR, NFPA, SOFT START. PLEX ISO


DWG. TYPE LAYOUT

DWG. NO. PXMI-LAS416

SHEET	SIZE
LA-1	B

PXMI-LAS416

REV	REVISION	DATE	ECN	NAME	CHKD
B-1	RELEASE TO PRODUCTION	05/16/25	PXEC0667	BTS	SEK

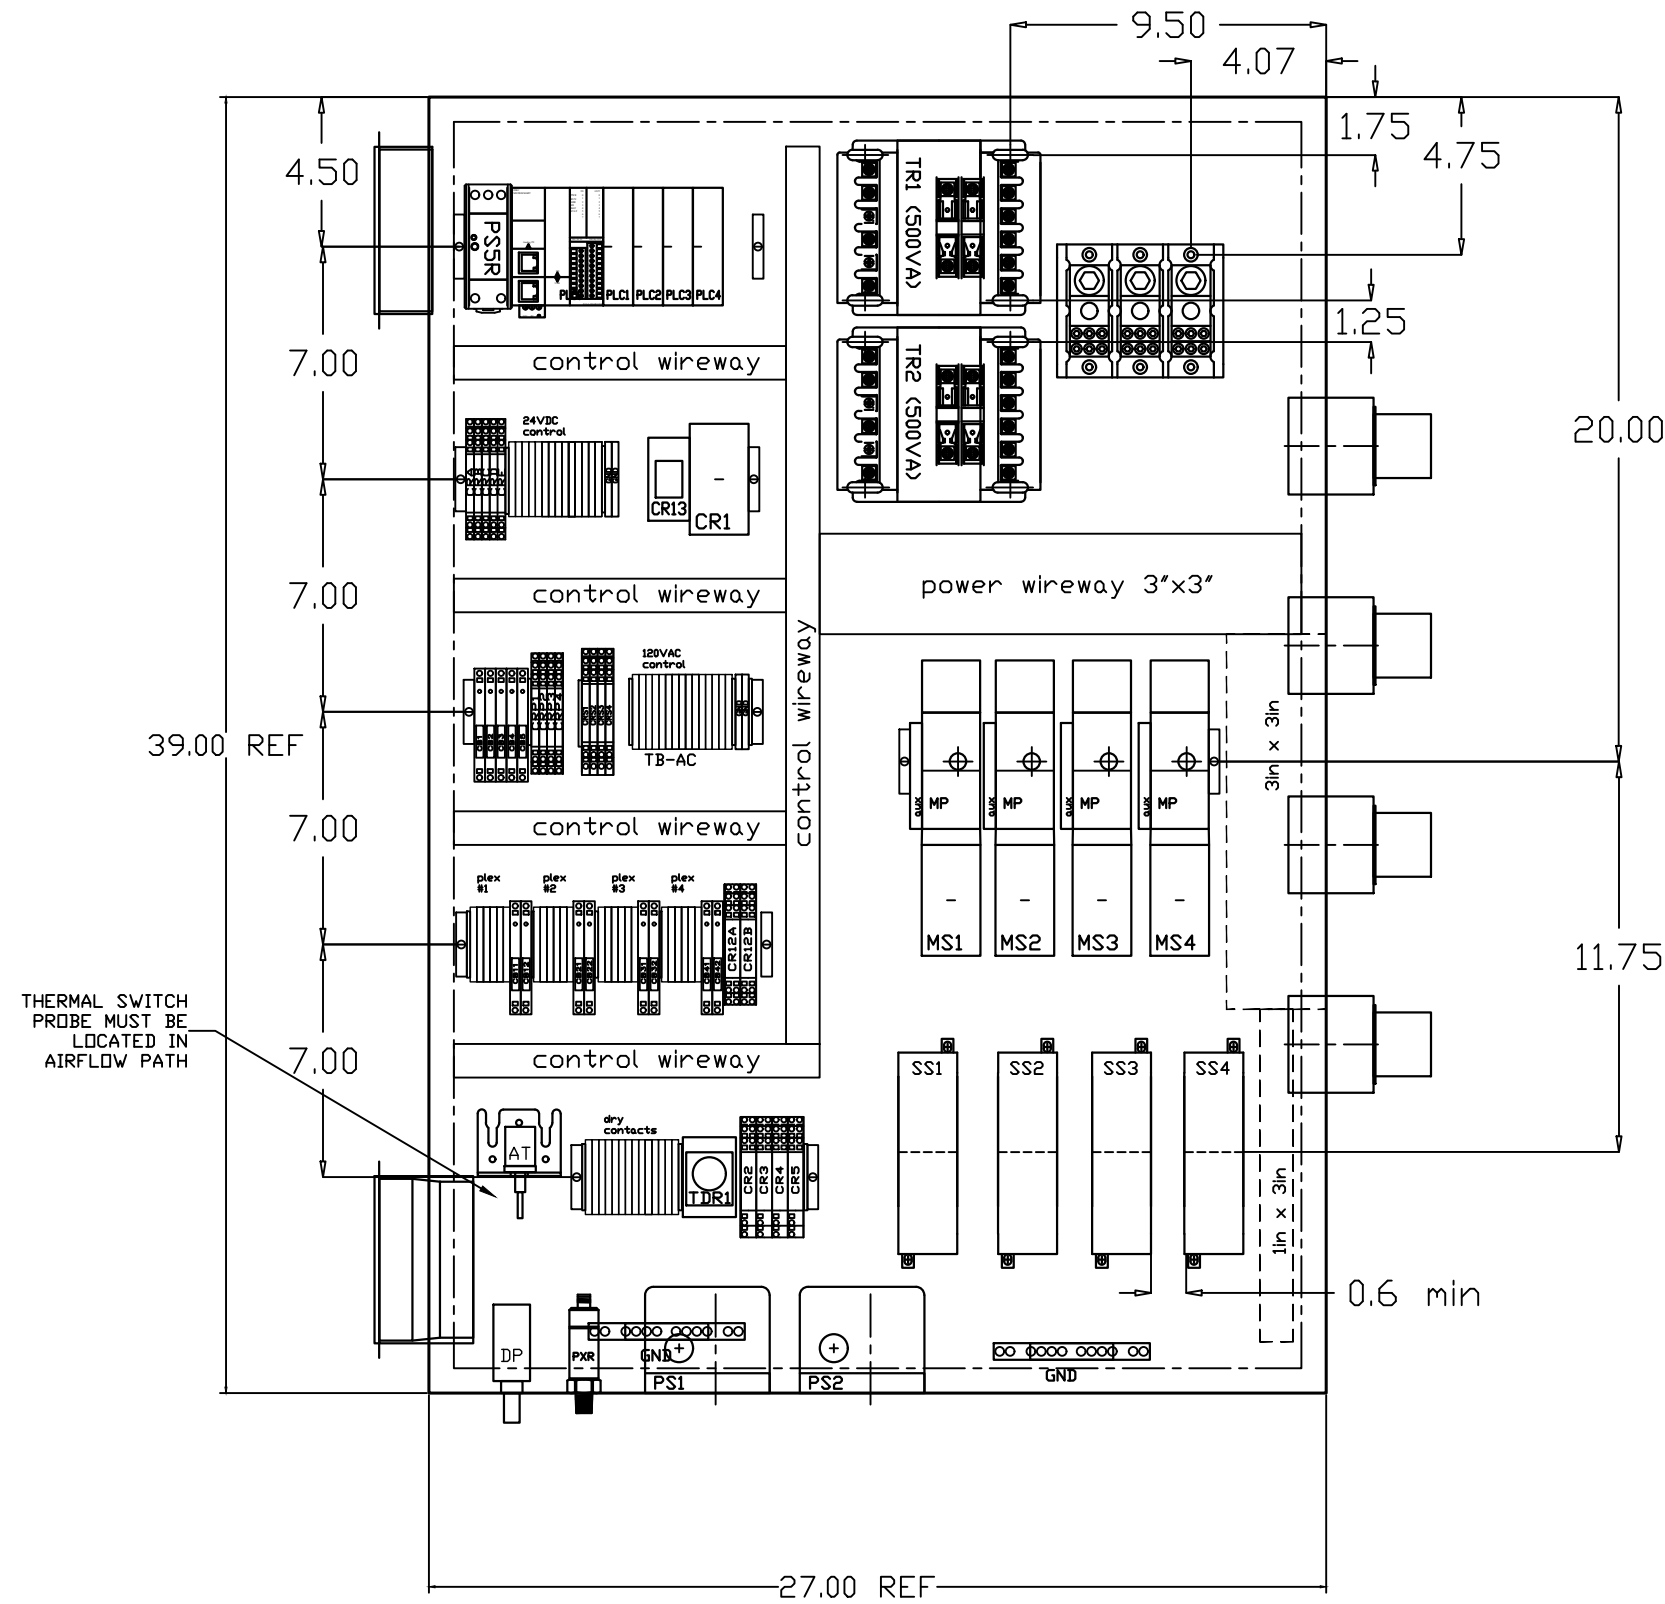

OPTIONAL:

POWEREX

CONFIDENTIAL DISCLOSURE:
This drawing is the property of POWEREX, INC. of Marmon Specialty Products and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
BTS	SEK	JRD
05/16/25	05/16/25	05/16/25

PANEL TYPE
QUADPLEX LAB COMP
HMI, BACNET, WEBSRV, NFPA, SOFT START. PLEX ISO

DWG. TYPE LAYOUT

DWG. NO.
PXMI-LAS416

SHEET	SIZE
LA-2	B

TABLE 1							REV	REVISION	DATE	ECN	NAME	CHKD
P/N							B-1	RELEASE TO PRODUCTION	01/14/15	PXEC0057	KMD	DMS
208V (3Ø)	72AJ	21.1	86.4	150	110	125						
	A2AJ	26.5	108	175	150	150						
230V (3Ø)	73AJ	17.9	73.6	110	90	110						
	A3AJ	24	98	150	125	150						
460V (3Ø)	74AJ	8.97	37.88	60	45	60						
	A4AJ	12	50	80	60	70						
380V (3Ø) 50HZ	78AJ	10.7	44.8	70	60	70						
	A8AJ	14.5	60	90	80	90						

NOTES:

1. RECOMMENDED TIGHTENING TORQUES FOR WIRE TERMINALS:
208-575 VOLT POWER 35 POUND INCHES
120 VOLT POWER AND CONTROL VOLTAGE 15 POUND INCHES

2. PANEL GROUND MUST BE CONNECTED TO EARTH GROUND

3. INSTALLER TO PROVIDE MAIN DISCONNECTING DEVICE FOR THIS ELECTRICAL ASSEMBLY. SHORT CIRCUIT PROTECTION IS RECOMMENDED. SEE TABLE 1. IF PROVIDING PANEL SHORT CIRCUIT PROTECTION USING TIME DELAY (CLASS J) FUSES, PANEL SCCR IS 65KA. OTHERWISE, PANEL SCCR IS 5KA.

4. ALL WIRES MUST BE LABELED ON BOTH ENDS

5. TRANSFORMER IS SIZED FOR LOADS SHOWN ON DRAWING ONLY. DO NOT CONNECT ANY OTHER DEVICES

6. △ -INDICATES A DRAWING WIRE CONNECTION TO ANOTHER PAGE.

7. SERVICE DISCONNECT USAGE - turn HOA switch to OFF position. Turn disconnect OF SAME UNIT to OFF position. Associated PLEX will be isolated for maintenance purposes. After completing maintenance, turn disconnect to ON position and return HOA switch to AUTO. This will return PLEX to normal operation.

CONTROL TRANSFORMERS - 500VA

REPLACEMENT	208	230	460	575	
FUSE TYPE	VOLT	VOLT	380 VOLT	VOLT	
FU1,2A FU1,2B	FNQR (CC)	6A	5A	5A	4A
FU3A,B	FNM	7A	7A	7A	7A

SEE XFRMR FOR CONNECTIONS

WIRE TYPE TABLE

VOLTAGE	WIRE NUMBERS	GAUGE	COLOR
120VAC	001-599,1100+	16-18AWG	RED/BLK
0VAC	W	16-18AWG	WHT/BLK
24VDC	600-1099	16-18AWG	PURPLE
0VDC	601	16-18AWG	PURPLE
GND	-	VARIES	GREEN
CUSTOMER SUPPLY	01-99	16-18AWG	YELLOW

SEQUENCE OF OPERATIONS

During normal operation the PBMI controller will signal the Lead compressor to run when pressure drops below lead cut-in set-point and stop when the pressure reaches the lead cut-out set-point. Lead alternation to the next pump, will occur with each lead run signal or every 10-minutes (which ever happens first). If demand cannot be satisfied by the lead pump, the lag pump(s) will start and stop based upon the lag cut-in and cut-out set-points. When more than one pump is running, lead alternation will occur when the lowest cut-out set-point is satisfied, or after 10-minutes (which ever happens first). The HOA switch’s place the pump in the following modes: Hand-turns pump on to run continuous. Off-disables pump from running. Auto-places pump in the “ready mode” and will start and stop based on sequence described above.

All plex configurations include a hardwired Back-up pressure switch circuit should a control failure occur. This circuit will call all pumps on and off based on the reserve pressure switch set-points.

Expandable systems include all control devices, operators, and programming for the maximum number of pumps (or plex) required. To expand the system: navigate to the “service screen” and enter the number of pumps.

Additional information and descriptions can be accessed through the HMI “service info” screen by pressing Sequence of Operations button.

OPTIONAL:

208V/230V/460V/380V

CONFIDENTIAL DISCLOSURE:
This drawing is the property of the CAMPBELL GROUP of the SCOTT FETZER COMPANY and subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.

DRAWN BY	CHECKED BY	ENGINEERING APPROVAL
KMD	DMS	DMS
01/14/15	01/14/15	01/14/15

PANEL TYPE

7. 5/10 SCROLL DATA
QUADPLEX PANEL DATA

DWG. TYPE MISC

DWG. NO.

DATA TABLE

SHEET	SIZE
D-1	B

SCROLL 7-10 QUADPLEX